

EXTRACTION CHROMATOGRAPHY

Technical Documentation - **New Developments**



Extraction Chromatographic Resins



Specialty Ion Exchange Resins



Novel Separation Materials



Method Development

INDEX

Company	3
Extraction Chromatography	4
Applications	5
<i>Extraction Chromatographic Resins</i>	<i>6</i>
CL Resin	6
CU Resin	8
DGA Sheets	9
ZR Resin	10
TK200 Resin	14
TK201 Resin	16
TK221 Resin	19
TK225 Resin	23
TK211/12/13Resins	25
TBP Resin	28
TK400 Resin	30
TK100/101 Resins	33
TK102 Resin	36
Guard Resin	38
TK-TcScintResin	39
Upcoming New Products	41
<i>Specialty Ion Exchange Resins</i>	<i>43</i>
TK202Resin	43
CS Resins	47
MnO ₂ -PAN Resin	48
<i>Sample Preparation</i>	<i>49</i>
Nucfilm Discs	49
Discs for alpha spec source preparation	49
References	51



TRISKEM INTERNATIONAL



Triskem International develops, manufactures and commercializes highly selective resins for the separation of a large variety of elements in numerous domains.

Triskem Resins are used for:

- the analysis of precious samples (environmental monitoring, radiation protection, bioassay)
- the recuperation of high value elements (production of radio metals for medical use and recuperation of their respective target materials and recovery of critical metals)
- the high precision determination of isotope ratios (dating/geochronology)
- the removal of particular elements before effluent release
- quality control of final and intermediary products in numerous industries including radiopharmacy

We also commercialize a complementary **range of accessories** such as vacuum box systems and products used for sample preparation like LSC cocktails, filters and discs for alpha spectrometry, and Pyrolyser systems for the determination of H-3, C-14, Cl-36, I-129,... in a variety of matrices including decommissioning samples.

Our technical support is carried out by a **worldwide recognized scientific team** consisting of radiochemistry PhDs who are amongst others members of the French nuclear equipment standardization agency (BNEN), ISO workgroups, and external IAEA experts and lecturers.

Triskem International products have now become a **standard technology** in the field of radiochemistry, geochemistry and radiopharmacy with methods used by accredited laboratories (Orano, BNFL, CEA, NNL,...) and regulatory organizations (IRSN, IAEA, BRGM,...) and many other customers working on radionuclide and element separation and purification.

EXTRACTION CHROMATOGRAPHIC RESINS

TrisKem International is an ISO9001 certified French independent company producing and developing extraction chromatographic resins.

Extraction Chromatographic Resins combine **the selectivity** of liquid-liquid extraction and **the rapidness and the ease** of use of chromatography.

Due to their high selectivity, methods using TrisKem's Extraction Chromatographic Resins, are shorter, demand less hands-on time and reduce, or even avoid, the use of toxic and dangerous reagents.

The resins are comprised of microspheric beads with a very high surface impregnated with an organic extractant. The large surface of the beads and the high content of extractant allow reducing the size of the columns, and therefore also the amount of reagents used – resulting in the generation of less waste.

Extraction Chromatographic Resins can be prepared using a wide choice of different extractants, and thus selectivities:

- Liquid anion exchangers
- Liquid cation exchangers
- Solvating and chelating extractants
- Macrocycles (e.g. crown ethers)
- Ionic liquids
- ...

Extraction Chromatographic columns, cartridges and discs are **facile to handle** and can easily be used in vacuum based systems or in automated separation setups e.g. for the separation of high active samples in glove boxes or hot cells, as for example needed for the preparation of radionuclides for nuclear medicine.



APPLICATIONS

Radiopharmacy

TrisKem manufactures selective resins for Lanthanides (e.g. Lu-177, Tb-161,...), Cu, Zr, Ga, Ac, Ge, Ti, Sc, Tc and many other radionuclides for medical purposes. We develop rapid, highly specific separation techniques for:

- Separation of radionuclides from irradiated targets
- Quality control of radionuclides for medical use
- Post-generator purification
- Radioprotection and Radioanalysis

Environmental Monitoring and Bioassay

TrisKem's extraction chromatographic resins allow the separation and determination of radionuclides (e.g. actinides and fission products) from bioassay samples and environmental matrices e.g. **soil, sediment, vegetation and seawater samples**. Their use allows a rapid and precise determination of radionuclides in emergency and routine situations, as well as, combined with suitable sample preparation methods, to obtain very low detection limits through analysis of large volume samples.

Decommissioning

The high selectivity of our resins not only allows the analysis of standard alpha and beta emitters (actinides, Sr-89/90, Ni-63, Tc-99,...) from high matrix samples including concrete, spent resin, but also the determination of so called difficult-to-measure (DTM) radionuclides such as **Sn-121m/Sn-126, Zr-93**,...

We are constantly working on developing new methods according to your needs. Methods for the following radionuclides are currently under development: **Se-79, Sb-125, Cs-135, Nb-93m/Nb-94, Ag-108m, Pd-107, ...**

Geochemistry and Metals Separation

TrisKem's expertise in separations and its variety of different resins with varying selectivities provides a number of opportunities to solve analytical problems through sample preparation. With our broad offer of products and long experience, TrisKem can help you meet lower detection limits with less uncertainty. The problems encountered are frequently centered on removing matrix that interferes with the instrumental measurement. ICP-MS is an example. Isobaric interferences often have to be removed in order to allow accurate determination of your analytes. Selectivity for the analyte of interest is important in these cases. Extraction chromatography is already widely used in various applications including **geochronology, isotope ratio determination and provenancing**.



A number of ready-to-use methods are available through our new website: www.triskem.com

CL Resin

The CL Resin is based on an extraction system that is selective for platinum group metals, gold and silver and is mainly used for the separation of chloride and iodide, especially in the context of Cl-36 and I-129 analysis, and the removal of radioiodine from effluents.

The selectivity for halides is introduced by loading the resin with Ag^+ allowing good selectivity for anions, especially halides, forming sparsely soluble or insoluble Ag complexes. Since the resin retains Ag^+ over a wide range of pH values it also allows loading chloride and iodide from various conditions (slightly alkaline to strongly acidic), ideally under reducing conditions to ensure their presence as halides.

Radioiodine is considered to be one of the most dangerous radioelements in terms of radiological effects in case of accidental release. Accordingly efforts are made to capture iodine from liquid effluents already during the production process before waste storage, to avoid a possible gas release from stored liquid waste at a later date.

Caroline Decamp of the Intitute of Radioelements (IRE) has developed a method for the removal of radioiodine from acidic (1M HNO_3) radioactive process waste solutions. The IRE combined the CL Resin with XAD-4 Resin and packed this mix (4g XAD-4 and 3g CL Resin) into columns. These mixed bed columns were then introduced into their process setup in order to remove radioiodine from their multi-curies production process solutions.

One prerequisite of the removal step was that it should not slow down the process; the radioiodine removal was thus tested at the same flowrates applied during the process. Flow rates up to $> 180 \text{ mL/min}$ and effluent volumes between 12L and 17L were tested, and it was found that under these conditions between 85 and more than 95% (overall mean retention yield for all solution volumes is $88\% \pm 5\%$ ($N = 14$, $k = 1$) of the radioiodine present were retained on the column, thus lowering the I-131 activity of the effluents by a factor of 10 from 100 GBq/L to about 10 GBq/L. 2000 GBq of I-131 could be removed per decontamination cycle and stored as solid waste.

Besides the removal of radioiodine from effluents the CL Resin is also used for analytical purposes. It allows for the preconcentration of I isotopes e.g. from waste water upfront to gamma spectrometry and, more importantly, for the determination of I-129 and Cl-36, both long-lived, volatile radionuclides, in environmental and decommissioning samples.

In case of analytical applications, after loading and rinsing of the resin (removal of matrix elements and interferents), chloride can be easily eluted from the resin using dilute SCN^- solutions whereas iodide remains fixed. Iodide can then be eluted from the resin using a moderately concentrated S^{2-} solution.

This allowed Zulauf et al. developing a simple scheme for the separation of chloride and iodide. The small elution volumes (5 mL) used for elution allow for direct measurement of the obtained fractions by liquid scintillation counting.

Warwick et al. have developed a method for the analysis of decommissioning samples (e.g. spent resin) based on the thermal decomposition of the sample to be analysed using a Raddec 'Pyrolyser' furnace. Volatilized chlorine species are transported by a stream of moistened air into a bubbler containing a 6 mM Na_2CO_3 solution where they are trapped. The authors modified the separation procedure so that the bubbler solution could directly be loaded onto a Ag^+ loaded CL Resin column.

It was observed that, since the sample was not loaded from a highly acidic sample solution, an additional rinsing step consisting of 5 mL 0.1M H_2SO_4 was necessary in order to improve C-14 decontamination.


Nottoli et al. employed the CL Resin for the determination of I-129 in spent resins by AMS. The authors first mineralized the resin via microwave digestion or by oxygen bomb combustion. Iodine was then purified on CL Resin using a modified purification method. Samples were prepared for AMS measurement by oxidation of the sulphide to sulphate with H_2O_2 , removal of the sulphate by precipitation with Ba followed by centrifugation, and finally an AgI precipitation.

With respect to its high selectivity for noble metals the CL Resin is currently being evaluated for use in Ag and Pd

Main applications






- Cl-36 and I-129 in water, environmental and decommissioning samples
- Removal of radioiodine from effluents

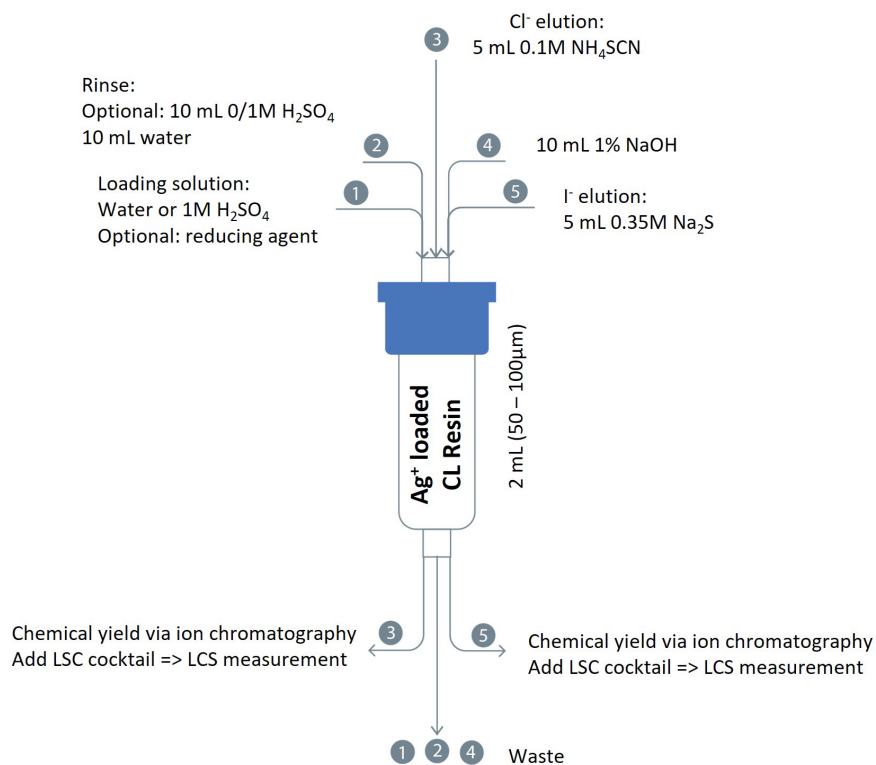

Scheme of chloride / iodide separations

Separation from 6 mM Na₂CO₃

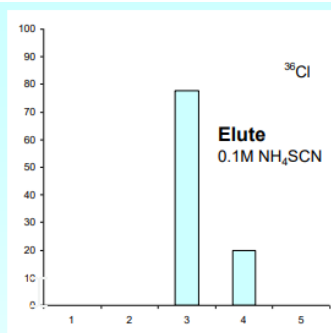

Cl recovery 98%

Example of a chloride / iodide separation

CU Resin



The CU Resin is used for the separation of Cu and is based on a Cu selective extraction system. The extraction behaviour of the CU Resin towards a number of elements in three different acids at varying acid concentrations is presented here.

Overall the resin shows high selectivity for Cu over all tested cations including Ni and Zn. Cu uptake is generally high at pH values greater than 2 while it can be easily eluted with mineral acids of elevated concentrations.


Further the resin shows high robustness against interference of elevated amounts of Zn and Ni, even at 1 g of Zn or Ni per g of CU Resin employed the $D_w(\text{Cu})$ remains greater than 1000.

A simple and fast method for the separation of Cu from irradiated targets was developed by Dirks. et al. allowing to obtain highly pure Cu in a very small volume (1 – 1.5 mL) in less than 10 min using a vacuum assisted separation setup.


It could be shown further that Cu can be concentrated and separated from other high-matrix samples such as sea water.




D_w of Cu and selected elements on CU Resin in HCl in varying pH values.



D_w of Cu and selected elements on CU Resin in HNO_3 in varying pH values.



D_w of Cu and selected elements on CU Resin in H_2SO_4 in varying pH values.




Elution study Cu spiked sea water sample on CU Resin.

Main applications



- Separation of Cu-64/67 from irradiated targets
- Concentration and separation of Cu from environmental matrices
- Purification of target materials


DGA Sheets




Radionuclide separation and radionuclidic purity determination was never easier. Separation of generator isotopes and radionuclide mixtures on DGA impregnated chromatographic paper, which has been developed at the CVUT, including mixtures like Ac-227/Th-227/Ra-223, Sr-90/Y-90, Ge-68/Ga-68, Mo-99/Tc-99m, Pb-212 and Ac-225/Bi-223 is now possible using one separation material, just by changing the composition of the mobile phase (diluted mineral acids like 1M HNO₃ or HCl). The chromatographic paper is impregnated with DGA with variable active compound loading (0.1-10%).

The method is easy to validate and TLC scanners or alternatively, after cutting the paper, common radiometers may be used to determine radionuclidic purity of a generator eluate or a purified radionuclide product.


Proposed standard sheet dimensions are 5 x 20 cm, 10 x 10 cm or 20 x 20 cm. Other formats and custom dimensions are however also available upon request.



Radiochromatogram measured immediately after separation



Radiochromatogram measured one hour after separation



Scheme of a chromatographic separation of a mixture of Ac-227 and its descendents. Th-227 remains on start, Ac-227 has a retention factor R_f of ca. 0.2, Pb-212 of ca. 0.7 and Ra-223 of ca. 0.9.




All data provided by J. Kozempel and M. Vlk, CVUT


ZR Resin

The ZR Resin is based on the hydroxamate functionality frequently used for the separation of zirconium, especially from Y target materials, for later use in radiopharmaceutical applications.

Dirks et al. characterized the resin with respect to its selectivity for selected elements in HNO_3 , HCl and oxalic acid; results are summarized in the following figures.

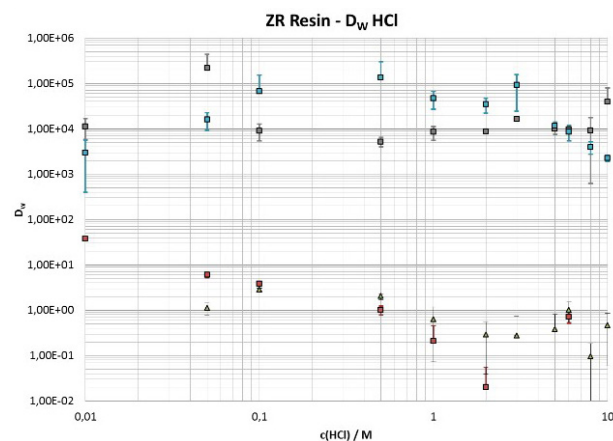

D_W values, ZR Resin, HCl , various elements




D_W values, ZR Resin, HCl , various elements


The ZR Resin shows high selectivity for Zr, Ti and Nb over a wide range of HCl concentrations (0.01M – 10M), Fe(III) is strongly retained at low and elevated HCl concentrations, retention is weak from 1 – 6M HCl . As expected, the resin shows very little selectivity for Sc and Y, a separation e.g. of Zr from Y and of Ti from Sc seems thus feasible.

The resin further shows quite interesting selectivity with respect to Ga and Ge.

Ga is very well retained at low HCl concentrations ($\leq 0.1\text{M}$) as well as at high concentrations ($\geq 5\text{M}$ HCl), while Zn e.g. is not retained at all. At HCl concentrations in-between, particularly at 1-2M HCl it is not retained. Ge on the other hand is very well retained at HCl concentrations $> 0.1\text{M}$. Especially at 2M HCl the selectivity for Ge over Ga is very high.




D_W values, ZR Resin, HNO_3 , various elements

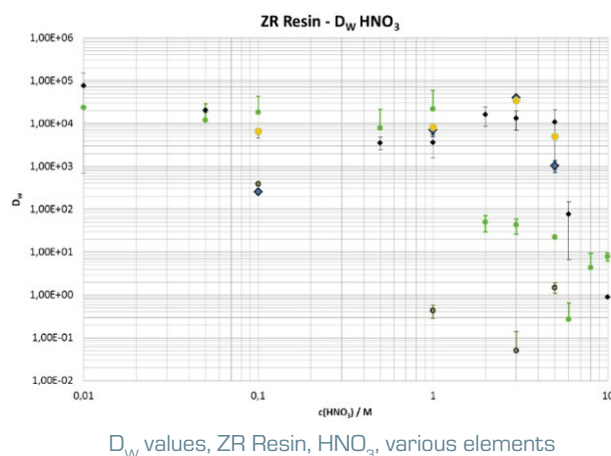

D_W values, ZR Resin, HNO_3 , various elements

The resin shows rather similar selectivity in HNO_3 . Zr, Ti and Nb are well retained up to 5M HNO_3 , Fe(III) is well retained up to 1M HNO_3 . At higher HNO_3 concentrations the nitric acid starts decomposing the extractant, as indicated by a colour change of the resin from white to brown; accordingly, the resin shows no significant selectivity towards the tested cations under these conditions. As in HCl , Y and Sc show no significant retention on the ZR Resin in HNO_3 .

It should be noted that the ZR Resin also shows high selectivity for Ge over Ga (and Ni/Co) at elevated HNO_3 concentrations.




D_W values, ZR Resin, HNO_3 , various elements

Oxalates are very strong complexing agents for Zr, accordingly they are very frequently used for the elution of Zr.

It could be shown that oxalic acid concentrations above 0.05M lower the D_w value of Zr on the ZR Resin strongly; they are thus suitable eluting agents for Zr. It was further observed that Nb shows rather elevated D_w values even at 0.05M oxalic acid, indicating that Zr and Nb may be separated by adjusting the oxalic acid concentration accordingly.


Based on obtained D_w values several elution studies were performed with main focus on the use of the resin in the context of radionuclide production for radiopharmaceutical use.

As indicated by the D_w values, the ZR Resin will retain Zr over a range of HCl concentrations. The rinsing conditions were kept close to the conditions suggested by Holland et al.: after loading the resin it is first rinsed with 4 x 2.5 mL 2M HCl, followed by an additional rinse with 4 x 2.5 mL water. Zr is finally eluted using 0.05M oxalic acid or higher.



Elution study ZR Resin, 100 mg, various elements, fractions analysed by ICP-MS

Under the given conditions a very clean separation of Zr from Y, Ti and Fe was obtained. Y and Fe are removed during the loading and rinsing of the ZR Resin, while Ti remains retained on the resin. Zr can be recovered quantitatively in ~2 bed volumes (BV) of 0.05M oxalic acid. High chemical yields could be obtained even in presence of up to 300 mg stable Y (using 100 mg ZR Resin).



Suggested method for the separation of Zr from Y targets (≤ 300 mg) using the ZR Resin.


The ZR Resin is currently also being tested for use in radioanalytical applications such as the quantification of Zr-93, as well as, in combination with the TK400 Resin, the separation of Fe/Nb/Mo, e.g. in decommissioning samples.

Another increasingly important use of the ZR Resin is the purification of Ga-68 from irradiated Zn targets. The production of Ga-68 via the irradiation of Zn-68 (as liquid or solid targets) on a cyclotron is indeed increasingly finding use as an alternative to Ge-68 generator produced Ga-68, as it allows frequent production of high activities.

As shown in the D_w value graphs the ZR Resin retains Ga very strongly in dilute HCl and HNO_3 , as well as in HCl of elevated concentration (≥ 5 M HCl). Zn on the other hand is not retained under any of these conditions. This selectivity allows its use for the separation of Ga-68 (and Ga-67) from irradiated Zn targets - liquid targets (typically dilute HNO_3) as well as solid targets (typically dissolved in HCl of high concentration).

HCl between 1M and 2M on the other hand is very suitable for Ga elution as its retention is particularly low under these conditions.


The following graph shows a typical example of such a separation. While Zn, and other typical impurities such as Cu and Ni, are not retained on the ZR Resin (in this example from high HCl) Ga is very well retained. A clean Ga fraction is then obtained by elution of Ga e.g. with 1.5M HCl.



Elution study, Ga separation on ZR Resin, various elements, fractions analysed by ICP-MS

This Ga-68 containing 1.5M HCl solution is too acidic for direct use in labelling or injection. Instead of converting the solution to more suitable conditions e.g. via evaporation and redissolution it is possible to use another resin for this step, the TK200 Resin. More information on the TK200 Resin selectivity may be found in its product sheet, in this context the most important fact is that it retains Ga well in the range of 1 - 2M HCl, while it allows for Ga elution in dilute HCl or water, making it very suitable for this required conversion.

It should be noted though that while other impurities like Cu are very well removed during load and rinse on the TK200 Resin, remaining traces of Zn are only partially removed, accordingly a clean separation on the ZR Resin upfront is very important, as can also be seen in the following elution study.



Elution study, Ga conversion on TK200 Resin, various elements, fractions analysed by ICP-MS

Several publications describe the use of the combination of ZR and TK200 Resins for the separation of Ga-68 from liquid Zn targets. The publication by Rodnick et al. is particularly interesting as it describes the use of a modified rinse on the TK200 Resin cartridge (2M NaCl/0.13M HCl) instead of the usual rinse with HCl. This allows for recovering the final Ga fraction at a better-defined HCl concentration during elution. The following scheme shows the separation method they




Fig. 4 Two-column approach for ⁶⁸Ga chemical separation


	Scheme A*	Scheme B
① ZR Load	< 0.1 M HNO ₃	
② ZR Wash	15 mL 0.1 M HNO ₃	
③ ZR Elution / Trapping on TK200	5–6 mL ~ 1.75 M HCl	
④ TK Wash	–	3.5 mL 2.0 M NaCl in 0.13 M HCl
⑤ TK Elution	H ₂ O	1–2 mL H ₂ O followed by dilute HCl to formulate

*Process as reported previously (Nair et al. 2017)

Scheme of Ga-68 separation from liquid Zn targets using ZR Resin and TK200 Resin, taken from Rodnick et al.


developed. Compared to liquid targets the irradiation of solid Zn targets allows for obtaining higher Ga-68 activities per production run. Thisgaard et al. describe the production of 194 GBq Ga-68 (at end of purification) as [⁶⁸Ga]GaCl₃ of high purity, and it's subsequent successful use for the labelling of PSMA-11 and DOATATE. The authors used a three-resin method for the separation. An additional LN Resin cartridge is used between the ZR Resin and the TK200 Resin to further remove potentially present impurities,

particularly Fe. The ZR Resin further shows very interesting selectivity for Ti, especially with respect to Sc. The graph below shows an example of a Ti/Sc separation performed on the ZR Resin, while Sc is not retained from 10M HCl Ti is fixed very well. 0.1M citric acid may then be used to elute Ti from the resin. However, the elution requires up to 10 bed volumes (BV) of the eluent or more. Beside citric acid, hydrogen peroxide or oxalic




Ti/Sc separation on ZR Resin [0.3 mL], fractions analysed by ICP-MS

acid of elevated concentration may also be employed. As Ti is retained over a very wide range of HCl concentrations, including dilute HCl, its potential for use as support for a Ti/Sc generator was also evaluated initially. In order to do so a 100 mg ZR Resin column (0.3 mL) was loaded with a small volume of a solution containing Ti and Sc. The column was then rinsed five times with 1 mL 0.01M HCl, followed by 10 rinses with 5 mL 0.01M HCl. Sc is easily removed in a small volume of dilute hydrochloric acid whereas Ti remains retained throughout the experiment, the general selectivity of a



Elution study on 100 mg ZR Resin, Ti and Sc, load from 0.01M HCl, repeated elutions, fractions analysed by ICP-MS


generator is thus given. Radchenko et al. examined the system in greater detail and using real, irradiated samples. They confirmed the ZR Resins selectivity for Ti over Sc, shown by the k_D



K_d values for Sc and Ti in HCl on ZR Resin, taken from Radchenko et al.

values the author obtained.


Based on these values they developed a separation method for the purification of Ti, to be more precise Ti-44, from irradiated Sc targets of elevated size (4 g). The



Ti/Sc elution profile on ZR Resin, irradiated 4g Sc target, taken from Radchenko et al.

graph below shows the elution profile they obtained. As may be seen a clean Ti separation from Sc was obtained. The Ti-44 was obtained as an HCl/H₂O₂ solution.

The authors used the purified Ti-44 solution for the preparation of two types of Ti-44/Sc-44 generators, one direct flow generator and, the preferred option according to the authors, one 'forward/reverse flow'



Schematic of a forward/reverse flow radionuclide generator, taken from Radchenko et al.

generator.

Especially the 'forward/reverse flow' generator showed very promising results with stable very low Ti breakthrough and high Sc elution yields. The obtained Sc-44 was successfully used to perform DOTA labelling with high yields, further indicating its high purity.

Malinconico et al. also used the ZR Resin to produce Ti-45 from irradiated Sc-45 targets.

Besides for the purification of Ga-68 from Zn targets the ZR Resin may actually also be used for the separation of Ge-68 from irradiated GaNi or GaCo targets. As discussed before, while Ga is very well retained at low mineral acid concentrations (typically $\leq 0.1M$) and at high HCl concentrations, it is not retained at medium high HCl and HNO₃ concentrations, and medium to high H₂SO₄ concentrations. Ge on the other hand is very well retained at elevated mineral acid concentrations. The D_w values show that especially between 1M – 3M HCl and HNO₃ the Ge retention is significantly higher than Ga retention.

It could be shown that the same is true for e.g. 5M H₂SO₄. The ZR Resin further shows no selectivity for Ni or Co under these conditions.

While the selectivity for Ge over Ga is very high in HCl its use for Ge separations is often avoided due to the high volatility of GeCl₄. In H₂SO₄ on the other hand Ge is not volatile, it further allows an efficient dissolution of typically employed target materials. Accordingly, a method for the separation of Ge-68 from multi gram irradiated GaNi or GaCo targets is currently being optimized.

The method is based on two subsequent purification steps on ZR Resin. First the dissolved target is adjusted to 5M H₂SO₄ and then loaded onto a 2 mL ZR Resin cartridge. After rinsing with 5M H₂SO₄ and purge with air for acid removal Ge is eluted with dilute citric acid. The Ge fraction is again adjusted to 5M H₂SO₄ and further purified on a 1 mL ZR Resin cartridge. Ge is once more recovered in dilute citric acid. In order to obtain the final product in dilute HCl (typically 0.05M HCl) the Ge is converted from citric acid to dilute HCl by adjusting it to 9M HCl, loading onto a Guard Resin cartridge, followed by elution with water or dilute acid. Further


Main applications



- Separation of zirconium
- Separation of gallium
- Separation of germanium
- Separation of titanium


TK200 Resin

The TK200 Resin is based on TriOctylPhosphine Oxide (TOPO) an extractant widely used in the extraction of metal ions.




Trioctylphosphine oxide (TOPO)

Some examples of D_w values determined in HNO_3 and HCl using ICP-MS are shown below.



D_w values of selected elements on TK200 Resin in HCl



D_w values of selected elements on TK200 Resin in HNO_3

D_w values for a wide range of additional elements may be found in the corresponding product sheet.


Cd, Zn and Ga are very well retained at HCl concentrations $>1\text{M}$. This is especially interesting with respect to Ga separation chemistry as Ga is not retained at 1 – 2M HCl on most resins.

In HNO_3 of the elements shown here only Ag is retained whereas e.g. Ga and Zn are not.

A typical example of the use of the TK200 Resin is the separation of Gallium isotopes (especially Ga-68) from irradiated Zn targets for medical use in combination with the ZR Resin.

ZR Resin is very well suited for the separation of Ga from Zn matrices, under low acid conditions (e.g. 0.1M HNO_3 often employed for liquid targets) as well as at high acid concentrations (e.g. 10M HCl) conditions often used for the dissolution of solid Zn targets.


An elution study showing the separation of Ga from Zn and potential impurities on ZR Resin is hereafter:



Ga/Zn separation on ZR Resin - load from 10M HCl


Ga is eluted from the ZR Resin in a small volume (1 – 2 column volumes) of 1.5M HCl, conditions too acidic for direct use in labelling reactions.

The TK200 Resin on the other hand allows for Ga extraction at 1.5M HCl, followed by Ga elution using aqueous solutions.



Ga elution from TK200 Resin with water following load from 1.5M HCl

It should be noted though that only very little additional Ga/Zn separation is taking place on the TK200 Resin.




D_w values of selected elements on TK200 Resin in HNO_3

Another typical application of the TK200 Resin is the determination of actinides such as U, Th and Pu in water samples.


As shown in the figure above, U and Th are very well retained over the whole HNO_3 concentration range, including 0.01M.

Elution of Th from 1g TK200 resin cartridge



Elution study Th retention and elution on TK200 Resin
(data courtesy of Nora Vajda)


Elution of U from 1g TK200 resin cartridge



Elution study U retention and elution on TK200 Resin
(data courtesy of Nora Vajda)


This allows for using the TK200 Resin for the preconcentration of actinides from acidified water samples, and their subsequent separation on the same column.

Elution of Pu from 1g TK200 resin cartridge




Elution study Pu retention and elution on TK200 Resin
(data courtesy of Nora Vajda)

U and Th are also very well retained from HCl.



D_w values of selected elements on TK200 Resin in HCl

By employing oxalic acid of suitable concentration a clean U/Th separation may be obtained as shown here:



Elution study U/Th separation on TK200 Resin

Main applications




- Ga separation for radiopharmaceutical applications (in combination with ZR Resin)
- U, Pu, Th concentration and separation

TK201 Resin

The TK201 Resin is based on a tertiary amine, it further contains a small amount of a long-chained alcohol (radical scavenger) to increase its radiolysis stability. The TK201 Resin rather acts as a weaker ion pair binding agent compared to the TEVA Resin, accordingly it is generally possible to elute under softer conditions.

Its main application is the separation of anionic species such as Tc(VII) or Re(VII).


The following graph shows the D_w values for Tc in HNO_3 and HCl.



D_w values of Tc on TK201 Resin in HCl and HNO_3 , obtained by LSC, data provided by N. Vajda (RadAnal)


Tc(VII) is very well retained at low acid concentrations. Its retention is generally significantly higher in HCl than in HNO_3 , even at elevated HCl concentration such as 2M it remains very strongly retained. In HNO_3 on the other hand its retention is rather low at concentrations above 2M.

The following graphs show the selectivity of the TK201 Resin for a wide range of elements in HCl and HNO_3 . All D_w shown in these graphs were obtained through ICP-MS measurements.




D_w values of selected elements on TK201 Resin in HCl

As expected, the TK201 Resin shows very high retention of Re(VII) in HCl even at rather elevated acid concentrations. Further Zn, Ga and Cu are retained, especially the latter allows for its use in radiopharmaceutical applications.




D_w values of selected elements on TK201 Resin in HCl, data provided by Russell et al. (NPL)

The TK201 Resin also shows strong retention of U and Pu at elevated HCl concentrations, both might subsequently be eluted in dilute acid.




D_w values of selected elements on TK201 Resin in HCl, data provided by Russell et al. (NPL)

The TK201 Resin further strongly retains Bi and Mo at elevated HCl concentrations, while other elements tested show no or only very low retention (Ru, Nb).



D_w values of selected elements on TK201 Resin in HNO_3 , data provided by Russell et al. (NPL)

The TK201 Resin generally shows rather limited selectivity in HNO_3 , similar to Tc(VII) Re is well retained at low HNO_3 concentrations (0.01 – 0.1M HNO_3). At elevated HNO_3 concentrations Pu is well retained and Th fairly well, other actinides are not retained under these conditions.




D_w values of selected elements on TK201 Resin in HNO_3 , data provided by Russell et al. (NPL)

Out of the other elements tested only Bi (at about 0.5M HNO_3) and Mo (at low HNO_3 concentrations) are retained. It is important to note that Mo is not retained at HNO_3 concentrations above 0.5M while Tc and Re are well retained (shown on the 1st figure), allowing for their clean separation.


It could further be shown by Vajda et al. that D_w values for Tc(VII) are very low in dilute NH_4OH : in 0.1M NH_4OH Tc(VII) shows a D_w of only ~2, accordingly it is easily eluted by $\geq 0.1\text{M}$ NH_4OH .

Additional elution studies indicated that an efficient Mo separation from Re is possible using 0.7M HNO_3 for Mo removal and dilute NH_4OH for Re elution.




Elution study, Re separation from various elements (incl. Mo and W) on TK201 Resin.

Vajda et al. could confirm that Tc is, like Re, not eluted in 0.7M HNO_3 , validating that Re is a good surrogate for Tc and thus also allowing an efficient Mo/Tc separation. Most suitable conditions for Tc elution were found to be NH_4OH greater or equal to 0.2M.




Elution study, Tc separation on 2 mL TK201 Resin cartridges, data provided by N. Vajda (RadAnal)

One of the main applications of the TK201 Resin is the separation of Cu isotopes (e.g. Cu-64) from solid Ni targets. Other than the CU Resin the TK201 Resin allows for Cu retention from high HCl (e.g. 6M), while letting Ni pass for subsequent recycling. Other potential impurities (e.g. Co) may be removed through rinses with 4 – 5M HCl. Cu may then be eluted in dilute HCl leaving Zn on the column.



Elution study, Cu separation on 1 mL TK201 Resin cartridges

In order to remove Fe and Ga impurities potentially present the dissolved Ni target (6M HCl) may first be loaded through a small TBP (or TK400) Resin cartridge which will retain both elements while letting Ni, Cu and Zn pass onto TK201 Resin for further purification. Cu may then be eluted from TK201 Resin e.g. in 0.05M HCl. This could be demonstrated i.e. by Svedjehed et al. The rinse with 5M NaCl/0.05M HCl is particularly noteworthy as it allows obtaining the final product in dilute HCl



Cu separation using TBP and TK201 Resins according to Svedjehed et al.

TK201 Resin may also be used to convert the Cu fraction eluted from the CU Resin (e.g. for the separation of Cu isotopes from Zn targets) from a highly acidic solution (e.g. 6 - 8M HCl) to conditions more suitable for labelling (e.g. dilute HCl). TK201 Resin will retain Cu e.g. from 6M HCl and can then be eluted with dilute HCl as shown e.g. by Kawabata et al. This will also ensure further Zn removal.

Main applications



- Separation of technetium
- Separation of rhenium
- Separation of Cu isotopes (incl. combined with CU Resin)




TK221 Resin

The TK221 Resin is based on a mixture of a diglycolamide and a phosphine oxide. It further contains a small amount of a long-chained alcohol and the organic phase is impregnated onto an inert support containing aromatic groups for increased stability against radiolysis.


The following graphs show the selectivity of the TK221 Resin for a wide range of elements in HNO_3 and HCl .

Out of the tested elements only Ca is weakly retained on the TK221 Resin in HNO_3 . Other alkaline, earth-alkaline elements and Al are not retained.



D_w values of selected elements on TK221 Resin in HNO_3

Y and Sc are very strongly retained from HNO_3 of elevated concentration. Fe(III) is also well retained at HNO_3 concentration $\geq 3\text{M}$ HNO_3 .




D_w values of selected elements on TK221 Resin in HNO_3

A wide range of transition metals such as Zn, Ga, Co, Ni and Cu are not retained from nitric acid.


The TK221 Resin generally retains tetravalent elements such as Zr and Hf at elevated HNO_3 concentrations.

The TK221 Resin shows very high retention of lanthanides at HNO_3 concentrations $\geq 0.1\text{M}$ HNO_3 , heavy lanthanides are even well retained in more dilute HNO_3 ($\geq 0.01\text{M}$). The retention of the lanthanides is significantly stronger than on TRU Resin.



D_w values of selected elements on TK221 Resin in HNO_3


U and especially Bi are well retained over the whole HNO_3 concentration range, while Th is well retained at $\text{HNO}_3 > 0.1\text{M}$. U retention is significantly higher than on other diglycolamide based resins such as DGA Resin. Pb and Sn are only weakly retained.



D_w values of selected elements on TK221 Resin in HCl

In HCl medium, none of the tested alkaline and earth-alkaline elements were retained on the TK221 Resin the same is true for Al.


Y and Sc are very strongly retained from HCl at elevated concentration ($\geq 2\text{M}$ HCl). Fe(III) is also well retained at HCl concentration $\geq 3\text{M}$.



D_w values of selected elements on TK221 Resin in HCl


Elements with a valency of +IV and higher such as Nb, Zr, Hf and Mo are very well retained at elevated HCl concentrations.

Other than many other transition metals, Zn and Ga are very well retained from $\geq 2\text{M}$ HCl. Both may be easily eluted in dilute HCl.



D_w values of selected elements on TK221 Resin in HCl

U, Sn and Bi are well retained over the whole HCl concentration range, while Th is only well retained at $\geq 3\text{M}$ HCl. Pb is generally only very weakly retained.




D_w values of selected elements on TK221 Resin in HCl


Lanthanides are generally very well retained at HCl concentrations $\geq 3\text{M}$ HCl, heavy lanthanides even at $\geq 1\text{M}$, and they may be eluted in dilute HCl.

One of the main applications of TK221 Resin is the concentration, purification and conversion of heavy lanthanides such as Lu from highly acidic solutions into dilute HCl (typically $\sim 0.05\text{M}$ HCl) conditions.

It allows e.g. to elute Lu in a smaller volume than DGA,N Resin. Accordingly, it may e.g. find use in the production of Lu-177.



Elution study, various elements on TK221 Resin



Elution study, various elements on DGA, normal Resin


A number of separation methods based on the TK221 Resin are currently being developed particularly for ca and nca Lu-177 purification, as well as the use of TK221 Resin as part of the separation of nca Lu-177 from up to 500 mg Yb-176.

The final product obtained using the TK221 Resin is typically additionally passed through a 1 mL A8 cartridge for trace nitrate removal.

Such a separation should also be applicable to the purification of Ac-225.

The fact that the TK221 Resin is showing higher U retention compared to e.g. DGA,N Resin might further allow for its use in a two column separation method for sequential actinides separation.

The following figure shows an elution study of various elements including U on TK221 Resin.




Elution study, various elements on TK221 Resin

U is very well retained under all employed HNO_3 and HCl concentrations and may finally be eluted in 0.1M oxalate. Am is expected to be eluted before U in dilute HCl.

With respect to the TK221 selectivity a stacked TEVA/TK221 method for the separation of U, Th, Pu, Am/Cm and Np seems very well possible.

In such a case Np(IV), Pu(IV) and Th(IV) would be retained, and separated, on TEVA while U and Am would pass through TEVA onto TK221 where both would be retained. It should then be possible to first elute Am with dilute HCl and finally U with dilute oxalic acid.


N. Vajda et al. developed such a method for the separation of Th, Pu, Am and U from water samples based on the TEVA/TK221 system. The development work was based on a typical Ca-Phosphate preconcentration step, and took into account the possible presence of Fe(III) originating from the oxidation state adjustment. Through a very thorough optimisation of the Am elution volumes a clean separation of Am and U on the TK221 could be achieved as shown below.



Th, Pu, Am and U separation on 2 mL TK221 Resin cartridge
[data courtesy of N. Vajda et al.]


Overall, the authors reported high chemical yields (92 – 106%) under the given conditions, and very good decontamination of the obtained actinide fractions (cross-contamination <1% respectively).

The developed separation protocol is summarized in the following figures.




Th, Pu, Am and U separation on TEVA/TK221 Resin, stacked cartridges [according to N. Vajda et al.]

The dissolved CaPhosphate precipitate is first passed through stacked TEVA and TK221 Resin cartridges. The cartridges are then rinsed with 3M HNO_3 to assure matrix removal and quantitative transfer of U and Am onto the TK221 Resin cartridge. Both cartridges are then separated: Pu and Th are separated on the TEVA Resin cartridge, while U and Am are separated on the TK221 Resin



Separation steps on split TEVA Resin cartridge
(according to N. Vajda et al.)




Separation steps on split TK221 Resin cartridge
(according to N. Vajda et al.)

When applying the developed method to the alpha spectrometric determination of tap and a sea water samples spiked with Th-230, Pu-239, Am-241 and U-233 they could confirm the clean separation of the actinides, as well as the fact that high chemical yields may be obtained.

Even for a highly charged matrix such as a sea water sample, chemical yields were in the order of ~90% for U, Pu and Am and ~70% for Th, only about 10 – 20% lower compared to the tap water samples (90 – 108%), making this a very promising alternative to the classical TEVA/TRU methods with the additional benefit of a more robust Am retention.


N. Vajda et al. further examined the TK221 Resin with respect to Ac retention.



Weight distribution ratios (D_w) of Ac on TK221 Resin.
Data courtesy of N. Vajda (RadAnal)

Overall, the D_w values for Ac are elevated in HNO_3 , even at very high (e.g. 8 - 10M) or low (e.g. 0.05M) concentrations. In HCl Ac retention is high at elevated HCl concentrations (9M HCl) while decreasing significantly at higher and lower acid concentrations. Especially at low HCl concentrations Ac D_w values are very low, indicating suitable elution conditions.


The high retention of Ac over a wide HNO_3 concentration range could further be shown through elution experiments.



Ac elution study on 1 mL TK221 Resin cartridge (100 – 200 μm), 10M HNO_3 rinse. Data courtesy of N. Vajda et al.

Other than the DGA Resins the TK221 Resin doesn't allow for Ac elution in 10M HNO₃, a step frequently used for Ac/Lanthanide separation. For TK221 Resin even higher HNO₃ concentration (12M HNO₃) is required.


Elution curve



Ac elution study on 1 mL TK221 Resin cartridge (100 – 200µm),

TK221 Resin does not allow, contrary to the DGA Resins, Ac elution in dilute HNO₃, dilute HCl is

Elution curve



Ac elution study on 1 mL TK221 Resin cartridge (100 – 200µm), 0.05M HCl elution. Data courtesy of N. Vajda et al.

required.

The fact that TK221 Resin retains Ac from dilute HNO₃ and allows its elution in dilute HCl might open the possibility of converting Ac solutions from dilute HNO₃ to dilute HCl using TK221 Resin.

It should be noted that TK221 Resin is now also available in 50 – 100µm particle size now, which allows for narrower elution.

Overall, a separation method similar to Lu-177 purification seems possible: Ac retention from elevated HNO₃, (or HCl) rinse with dilute HNO₃ to remove impurities and lower HNO₃ concentration on the resin, followed by elution in HCl. Ideally the final product should be loaded through a small anion exchange resin cartridge (e.g. 1 mL A8 Resin) to remove last traces of nitrate.

Additional work on the Ac separation on TK221

Main applications




- Separation and concentration of lanthanides (e.g. ca and nca Lu-177)
- Separation of actinides
- Separation of actinium

TK225 Resin

The TK225 Resin is based on a mixture of a diglycolamide and an ionic liquid. The organic phase is impregnated onto an inert support containing aromatic groups for increased stability against radiolysis.


The main application of the TK225 Resin is the removal of radiolanthanides from acidic solutions, particularly from solutions of elevated HNO₃ concentration, for decontamination purposes.

The following graphs show the selectivity of the TK225 Resin for a wide range of elements in HNO₃ and HCl. All D_w shown in these graphs were obtained through ICP-MS measurements.




D_w values of selected elements on TK225 Resin in HNO₃

Out of the tested elements only Ca is quite strongly retained at elevated HNO₃ concentrations. Sr and Pb, too are retained under these conditions to a lesser extent though.




D_w values of selected elements on TK225 Resin in HNO₃

Lanthanides, especially heavy lanthanides, Y and Sc are very strongly retained from HNO_3 of elevated concentration. Especially for heavy lanthanides the D_w values remain very high, even at low HNO_3 concentrations.




D_w values of selected elements on TK225 Resin in HNO_3

The TK225 Resin generally retains tetravalent elements such as Zr, Hf and Th at elevated HNO_3 concentrations quite strongly.



D_w values of selected elements on TK225 Resin in HCl


The TK225 Resin shows elevated retention of Ca and Zn at high HCl concentrations. Other elements shown are not or only very weakly retained.



D_w values of selected elements on TK225 Resin in HCl

Especially heavy lanthanides are well retained over a broad HCl concentration range, with highest retention being observed at high HCl concentrations.

At high HCl concentrations Y, Sc and lighter lanthanides are well retained, too.



D_w values of selected elements on TK225 in HCl

Higher valent elements such as Sb, Sn, Zr and U are well retained at high HCl concentrations, while showing very little retention at low HCl concentrations. TK225 Resin is mainly used for the removal of radiolanthanides, especially heavy radiolanthanides such as Lu-177, Yb-175, Tb-161,... from acidic solutions.

Especially the heavy lanthanides are near impossible to elute, accordingly the resin is mainly suitable for the decontamination of acidic effluents and waste solutions.

Main applications

- Lanthanides removal from acidic effluents



TK21 1/2/3 Resins

The TK211, TK212 and TK213 Resins are based on different mixtures of organophosphoric, organophosphonic and organophosphinic acids. It could be shown that under certain conditions and for certain lanthanide pairs, such mixtures can show increased selectivity compared to the respective pure compounds.

The organic phase further contains a small amount of a long-chained alcohol that will act as radical scavenger to increase the radiolysis stability of the resin.

The inert support onto which the organic phase is impregnated contains aromatic groups which will also contribute to the increase of the radiolysis stability of the resins.

The inert support further shows an elevated capacity for the extractants. Accordingly, this allows the TK211/2/3 Resins to have a higher extractant load compared to e.g. the LN Resin series.

The TK211/2/3 Resins show, like the LN Resins differences in their respective acidities. TK211 Resin is the most acidic resin, accordingly it will extract lanthanides, and other elements, at higher acid concentrations than e.g. TK212 and TK213 Resins. TK212 Resin on the other hand is more acidic than TK213 Resin (order of acidity: TK211 > TK212 > TK213).

The selectivity and retention of the lanthanides is generally very similar in HNO_3 and HCl on all three resins, accordingly both acids may be employed for the separation of lanthanides.

This difference in the relative acidity of the resins can be exploited to facilitate otherwise more complex lanthanide separations.

This will particularly be the case for the separation of very small amounts of one lanthanide from a large excess of its neighbouring lanthanide.

Typical examples are the production of nca Lu-177 (separation from irradiated Yb-176 targets) and nca Tb-161 (separation from irradiated Gd-160 targets).

By performing a first separation on a 'less acidic resin' such as TK212 Resin followed by direct elution of the lanthanide fraction to be further purified onto a more acidic resin such as TK211 Resin for further purification ("sequential separation") it is possible to eliminate intermediary steps such as the use of TK221 (or DGA) Resin to convert the lanthanide fraction from higher acid concentration to low acid concentration.

In an ideal case even a fully sequential three column separation might be possible (TK213 => TK212 => TK211).


Two examples of the use of such sequential separation steps will be shown in the following.

The production of nca Lu-177 is rapidly gaining importance due to its increased use in nuclear medicine. Reliable, preferably easy to automatize methods that allow for its separation from irradiated Yb-176 targets of elevated size (≥ 500 mg) are thus of increasing importance.

Horwitz et al. describe a method based on three LN2/DGA cycles for the separation of nca Lu-177 from 300 mg Yb-176 targets. While this method gives good yields ($\sim 73\%$) in a short separation time (~ 4 h) the fact that an elevated number of columns are required complicates its automatization. Further it has only been tested for up to 300 mg of target material.

By introducing a sequential separation step this method can be partially simplified.

It could be shown that the method described in the following figure allows for separating Lu from up to 500 mg of Yb with elevated Lu recovery ($\sim 85\%$) and a very low amount of residual Yb in the final Lu fraction.

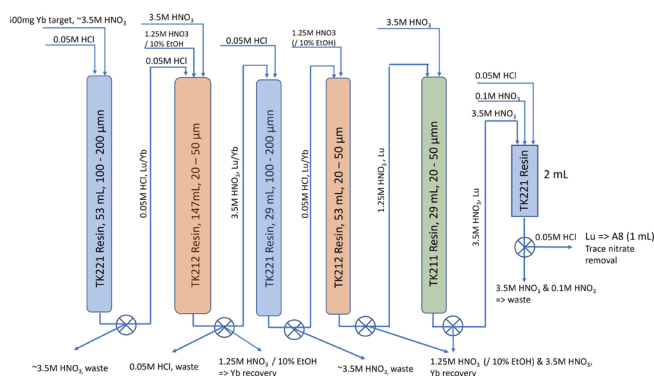


Scheme of a method for the separation of Lu from 500 mg Yb using TK212, TK221 and TK211 Resins

The increased Lu recovery is, other than the use of TK212 Resin instead of LN2 Resin, also due to the adjustment of the eluting agent used for the chromatographic separation of Lu and Yb on the first TK212 Resin column from 1.3M HNO_3 , as suggested by Horwitz et al., to 1.25M HNO_3 / 10% EtOH.

It should be noted that adding EtOH only showed an improvement for the 1.25M HNO_3 but not for the 3.5M HNO_3 . Further, mixing 3.5M HNO_3 with EtOH should be strictly avoided for safety purposes.

The following figures show typical chromatograms obtained during the separation of Lu from 500 mg of Yb (initial Lu:Yb ratio: 1:1000). All experiments were performed using stable elements, fractions of defined sizes were collected, diluted, and analysed off-line by ICP-MS. Relative recoveries were calculated for Lu and Yb and plotted against the elution volume.




Example of a Lu separation from 500 mg Yb on a TK212 Resin column [2.5 x 30 cm, 147 mL] using 1.25M HNO₃ / 10% EtOH and 3.5M HNO₃

It should be noted that the switch to 3.5M HNO₃ in the given example was made at a rather late stage of the separation. In the final version of the process it should take place earlier, ideally triggered via radiation detection, close to the chosen cut-off point (left end of the green frame).

Indeed, the moment of the switch will have, especially on the first column, a considerable influence on the Lu recovery and Yb carry-over. This is mainly due to the significant tailing introduced by the macro-amount of Yb.

The fractions comprised in the green frame ("Lu fractions") were combined and passed through a 5-10g TK221 Resin cartridge for conversion to ≤ 0.05 M HCl. The Lu fraction thus obtained in dilute HCl was then loaded onto the next TK212 Resin column (1.5 x 30cm, 53 mL).


Due to the lower of amount of Yb present on the column the tailing of the Yb and Lu elution is less pro-



Example of a Lu separation, fraction obtained from a first TK212 separation, containing 94 mg Yb, on a second TK212 Resin column [1.5 x 30 cm, 53 mL] using 1.25M HNO₃ / 10%

Although this would be possible, in this example the Lu containing fractions (green frame) are not eluted in HNO₃ of elevated concentration (as described in the Horwitz method), passed through a TK221 (or DGA) Resin cartridge and eluted in dilute HCl for another load onto TK212 Resin.

Instead the combined fractions are directly loaded onto a TK211 Resin column (1.1 x 30 cm, 29 mL) for the final



Example of a Lu separation fraction, obtained from the second TK212 Resin separation from <1 mg Yb, on a TK211 Resin column [1.1 x 30 cm, 29 mL] using 3.5M HNO₃

Lu is finally obtained following separation/elution e.g. with 3.5M HNO₃.

As final step the obtained Lu fractions (as indicated in the green frame) were combined and loaded onto a 2 mL TK221 cartridge, any last potentially present impurities are removed through consecutive rinses with 3.5M HNO₃ and 0.1M HNO₃. Lu is then finally eluted using ≤ 0.05 M HCl.

Last traces of nitrates that might still be present will be removed via a 1 mL anion exchange cartridge (A8 Resin).


A further upscale of this separation process to 1000 mg Yb is being finalized.

Another radiolanthanide increasingly finding use is Terbium. As Tb isotopes may be used for PET imaging (Tb-152), SPECT imaging (Tb-155), alpha therapy (Tb-149) and beta therapy (Tb-161) it is also referred to as the 'swiss army knife' of nuclear medicine.

Particularly the interest in Tb-161 is currently increasing significantly, accordingly methods for the separation of Tb from irradiated Gd targets of elevated size are needed.

The development, and later upscale, of methods for the separation of Tb from 500-2000mg Gd is currently ongoing. The next figure shows a scheme of a suggested separation process.

As may be seen the separation is more straightforward compared to the separation of Lu from Yb targets.

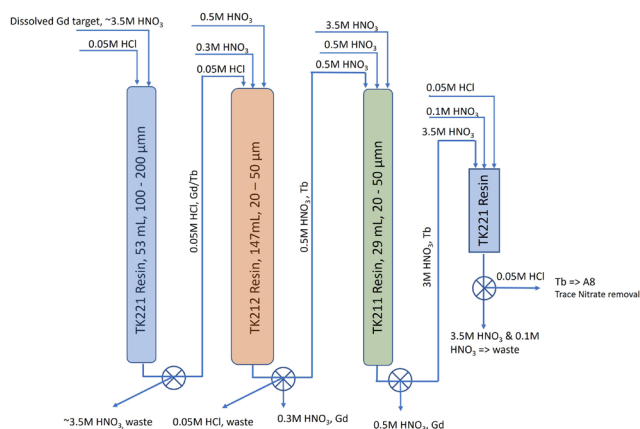

Scheme of a method currently under development for the separation of Tb from 1000 mg Gd using TK221, TK212 and TK211 Resins

The following two figures show typically obtained chromatograms (stable Gd, Tb and Dy, with an original ratio of 1000:1:1).


Like for the Lu separation the separations were performed using stable elements, fractions of defined volumes were taken and analysed by ICP-MS.

A first separation is performed on a TK212 Resin column. This step allows for an initial separation of Tb from Gd and Dy.

The obtained Tb fractions (indicated by the orange frame) were then combined and directly loaded onto a TK211 Resin column for final purification of the Tb.


As may be seen in the next figure under the chosen conditions most of the Gd is breaking through during the load, any Gd remaining on the columns is rinsed of with 0.5M HNO₃.

It could be shown for the Lu separation process that the addition of small amounts of EtOH (10% v/v) improves the separation, this is currently also being tested for the Tb separation.



Example of a Tb separation from 1000 mg Gd on a TK212 Resin column (2.5 x 30 cm, 150 mL) using 0.3M HNO₃ and 0.5M

Increasing the concentration of the mineral acid (in this example to 0.75M HNO₃) will lead to the elution of Tb, leaving potentially remaining traces of Dy on the columns. In case the presence of Dy can be ruled out this elution can be performed at higher acid concentrations, thus lowering the elution volume.



Example of a Tb separation from 500 µg Gd on a TK211 Resin column (1.1 x 30 cm, 150 mL) using 0.5M HNO₃ and 0.75M

As a final step the Tb will be concentrated on a 2 mL TK221 Resin cartridge, any last potentially present impurities are removed through consecutive rinses with 3.5M HNO₃ and 0.1M HNO₃. Tb is finally eluted using ≤0.05M HCl.

Last traces of nitrates that might still be present will be removed via a 1 mL anion exchange cartridge (A8 Resin).

The indicated method is currently undergoing further optimisation and upscale.


Prepacked TK211/212/213 Resin columns of various sizes (e.g. 375 mL, 147 mL, 53 mL and 29 mL) are commercially available.

Main applications

- Lanthanide separation e.g. nca Lu-177 and nca Tb-161



TBP Resin




TriButylPhosphate [TBP]

The TBP Resin is comprised of an inert support impregnated with Tributylphosphate (TBP). TBP is a widely used extractant, it finds for example application in the Purex process, the reprocessing of U and Pu from spent fuel. Other applications include, amongst others, the separation of yttrium for analytical purpose.

The following figure shows the D_w values of selected actinides on the TBP Resin in HNO_3 and HCl.

Vajda et al. also evaluated the influence of Fe(III) and three anionic interferences (oxalic, sulfuric and phosphoric acid) on the U and Pu uptake.




In 8M HNO_3 a Fe concentration of 0.1M is not interfering with the uptake of U(VI) and Pu(IV), the same is true for Np(IV) and Th(IV). Unlike this, the same Fe concentration very strongly interferes with the retention of U and Pu in 9M HCl.

Oxalates show no interference with the U uptake even at concentrations of up to 0.5M. Sulfate, and especially phosphate, interfere significantly when present in elevated amounts. In general the actinides show an increasing retention at increasing acid concentrations.



However, of all actinides, only Pu shows D_w values higher than 100 in HNO_3 , whereas the other actinides peak at D_w values between 60 and 80. Pu is even stronger retained at high HCl concentrations ($D_w > 1000$ on 9M HCl), retention of the other actinides, with exception of Np in 9M HCl ($D_w = 140$) is rather low, especially Th(IV) shows very little affinity to the TBP Resin.

Nora Vajda et al. could show that the TBP Resin can be used for the separation of Pu from other actinides and developed a method for its use for the determination of Pu in water samples.

The Pu(IV) extraction from 9M HCl is very robust, although the tested anions do interfere with its uptake when present in concentrations $\geq 0.1\text{M}$, the D_w values of Pu still remain greater than 500.



D_w values of selected actinides in HNO_3 and HCl media on TBP Resin



D_w values of selected elements on TBP Resin in HCl and HNO_3

The TBP Resin has further been characterized with respect to the uptake of various elements in HNO_3 and HCl .

Beside Pu(IV) and Np(IV) several other elements such as Au , Hf , Fe , Sn and Ga also show high affinity for the TBP Resin in HCl .

While Au remains retained under all tested conditions, making its elution rather difficult in HCl , the other elements only show high D_w values at elevated acid concentrations, and low D_w values at lower concentrations.

In 1M HCl for example only Sn shows elevated D_w values whereas Fe , Ga , Sb ... show very little affinity to the resin, allowing for its separation from these elements. Sn can then be eluted e.g. with 0.1M HCl .

The TBP Resin generally shows very good selectivity for Sn over Te (Te-126 is an isobaric interference for the mass spectrometric determination of a long-lived beta emitter Sn-126 , frequently determined in decommissioning and radioactive waste samples) and Cd which is frequently used as target material for the production of Sn-117m , a conversion electron emitter used in nuclear medicine. The resin also shows interesting selectivity for Sb , however its oxidation state needs to be carefully controlled.

In HNO_3 of all tested elements only the actinides (at elevated HNO_3 concentrations), and Ag (at low HNO_3 concentrations), are retained on the resin. Based on the obtained data, Dirks et al. have developed a procedure for the separation of Sn from various elements.

Most of the tested elements are not retained during load and first rinse. Sn and part of the Ga and Fe are retained. The latter two are first removed with 1M HCl , Sn is then quantitatively eluted with $6\text{ mL } 0.1\text{M}$

HCl in high purity. For samples containing elevated amounts of Fe it will be necessary to either remove Fe before loading (e.g. by anion exchange) or to assure complete reduction of Fe to Fe(II) .

Main applications




- Separation of tin
- Separation of zirconium
- Separation of scandium
- Separation of actinides




TK400 Resin

The TK400 Resin is an extraction chromatographic resin that is comprised of octanol impregnated onto an inert support. Knight et al. showed that long-chained alcohols, especially octanol, show very interesting selectivity towards Pa at high HCl concentrations, allowing for facile Pa/Np separation using column chromatography. Jerome et al. characterized a number of elements including Pa, Np, U and Th.




D_w values of selected elements on TK400 Resin in HCl at varying concentration [Data provided by Ivanov et al]

They found that Pa retention sharply increases at high (≥ 9 M) HCl concentrations whereas other elements tested are not retained. At HCl concentrations < 8 M HCl on the other hand D_w values of Pa were found to be low allowing for its elution in a small volume. Ostapenko et al. found a similar trend for Pa retention with k' values being high for Pa at high HCl concentrations (9M). These results correspond overall well to the selectivity observed by Knight et al. when performing Np/Pa separation.

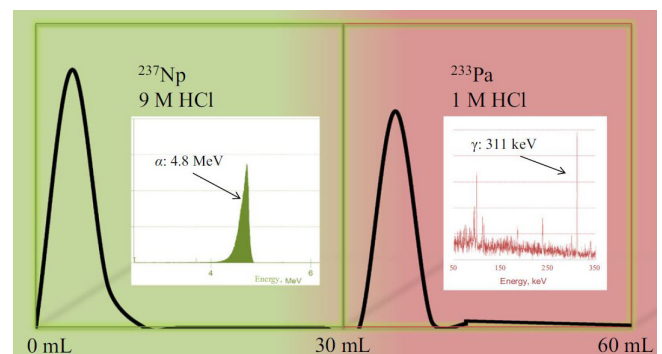


Elution study, Np/Pa separation on long-chained alcohol resin
[Taken from Knight et al.]

The resin shows high selectivity for Nb at high HCl concentrations over other elements tested such as Ta, Zr, Hf and lanthanides which are not, or only very poorly as in the case of Ta, retained by the resin.




D_w values of selected elements on TK400 Resin in HCl at varying concentration




Elution study, Nb separation from selected cations, 2 mL TK400 Resin column

With respect to its selectivity the TK400 Resin shows the potential for allowing a number of interesting separations such as Nb/Zr and Pa/U/Th. The results of an elution study on the separation of Nb from a number of elements, including Zr, and the separation method used to obtain these results are shown in following figures. Jerome et al. employed the TK400 Resin for the separation of Pa from its descendants following the procedure shown here. They found that U, Th, Ac, Ra and Pb were removed from the resin during load and rinse, allowing for obtaining a clean Pa fraction with high chemical yield (environ 83%).




Pa separation on TK400 Resin



Nb separation on TK400 Resin


Another interesting application of the TK400 Resin was described by Tieu et al. and Svedjehed et al. Both authors used the TK400 Resin for the separation of Ga-68 from irradiated solid Zn targets. Svedjehed et al. showed that it is advantageous for solid targets to use the TK400 Resin instead of ZR Resin in combination with A8 and TK200 Resins.

The fact that the TK400 Resin shows higher Fe capacity than e.g. TRU Resin makes its use in the analysis of i.e. decommissioning samples interesting. A method combining the use of the TK400 Resin (separation of Fe, Nb and Mo from most matrix elements) and ZR Resin (subsequent separation of Fe from Nb and Mo) is currently being optimized. The following graphs show typically



Fe/Nb/Mo separation from selected elements,
TK400 Resin

As may be seen, while Fe, Nb and Mo are well retained a large number of other elements, such as e.g. Zr, U, Th, Cs, Co,... are removed during load and rinse. These three elements may then be eluted in dilute HCl and directly loaded onto ZR Resin for further separation.



Fe, Nb and Mo separation on ZR Resin


The fact that the TK400 Resin shows high selectivity for Fe and Nb but not for Zr may also allow its use in the separation of Zr-89 from solid Y targets, with the aim to further lowering the amount of these impurities in the final product.

First tests showed that loading a simulated dissolved target solution containing Zr, Y, Nb and Fe through a TK400 Resin cartridge at 9M (or 10M) HCl, followed by a rinse under the same conditions will allow retaining Nb and Fe on the TK400 Resin while Zr (and Y) will pass through. Combining the load and rinsing fractions containing Zr, adjusting them to 11M HCl and loading this solution through a TBP Resin cartridge (similar to the method described by Graves et al.) will then allow a clean Zr separation with high chemical yield. It should be noted that alternatively 10M HCl may be used as loading condition on both cartridges.


This could simplify the separation, as the intermediate HCl concentration adjustment is not

necessary. It might further allow for the use of stacked cartridges in the initial loading step, this modification will require further testing though. Zr is finally eluted from the TBP Resin cartridge using dilute HCl.

If desired, Nb and Fe may be recovered from the TK400 Resin cartridge using dilute HCl. The graphs below show typically obtained elution studies



Nb and Fe removal from Zr (and Y)
on a 2 mL TK400 Resin cartridge



Zr purification on a 2 mL TBP Resin cartridge

Main applications



- Separation of protactinium
- Separation of gallium
- Separation of iron
- Separation of niobium


TK100 Resin & TK101 Resin

Crown-ether based extraction chromatographic resins such as the SR and PB Resins are frequently used for the separation and determination of Sr-90 and Pb-210 in aqueous samples via liquid scintillation (LSC) or gas proportional counting (GPC).

These resins only show significant Sr and Pb retention at moderate to high acid concentrations; thus not allowing for direct loading of the analytes from filtered raw or acidified water samples.

TK100 Resin

The TK100 Resin consists of a crown-ether with high selectivity for Sr and Pb and HDEHP a liquid cation exchanger.




Jake Surman from Lancaster University characterized the resin with respect to D_w values of Sr at different pH values \geq pH 2, as well as at HNO_3 and HCl concentrations higher than 0.01M. It could be shown that the resin shows high D_w values for Sr at pH values up to 8 ($D_w \gg 100$).

As shown in the following figure, the Sr uptake at pH 2 is high, especially in HNO_3 . The latter fact is of importance as water samples are often acidified to pH 2 using HNO_3 directly after sampling in order to stabilize them for storage before analysis.

At elevated HNO_3 concentrations the resin shows an increase of the Sr D_w values to about 100 at 8 – 10M HNO_3 . The TK100 Resin is thus behaving very similar to the SR Resin under these conditions. This makes the additional use of pre-concentration steps such as ion exchange or co-precipitation necessary.

In order to simplify the Sr-90 and Pb-210 separation, two new extraction chromatographic resins with an extended uptake pH range were developed, allowing for direct loading of water samples (pH 2 – 8) and the subsequent purification of the analytes on the same column.



D_w values Sr and Y on TK100 Resin, varying HNO_3 and HCl concentrations

As Sr elution with water or dilute nitric acid is not possible, a number of other eluting agents were tested and 2M HCl, 3M HCl and 0.1M EDTA were found to be most suitable of all tested.

Several other elements also show an affinity to the TK100 Resin at pH 7, making separation chemistry necessary in order to obtain a clean Sr fraction.

The influence of several typical matrix elements on its uptake onto the TK100 resin at pH 7 was tested. Even though high salt contents indeed interfere with Sr uptake, even at NaCl concentrations of 500 mM, K concentrations of 400 mg/L, Mg concentrations of 1300 mg/L and Ca concentrations of 500 mg/L the D_w values for Sr remain greater than 100.

Surman et al. could further show through elution studies that the resin allows for the separation of Sr from a number of elements such as Ca, K, Mg.

Even if the limiting concentrations will be lower for combinations of the interferences, the resin seems well suited for surface and especially drinking waters.


Surman et al. could further show through elution studies that the resin allows for the separation of Sr from a number of elements such as Ca, K, Mg, Ba, Co, Am, Cs and Pb. It should be noted that Pb is not eluting under the chosen conditions.

Additional studies performed by Dirks et al. with 1L samples at pH 7 loaded onto a 2 mL TK100 Resin column in aliquots of 100 mL at a flow rate of 5 mL/min showed that K and Ca breakthrough during load without being retained.

Unfortunately Sr breakthrough starts occurring after a loading volume of approx. 600 mL indicating that the maximum sample volume to be loaded onto the 2 mL column for Sr analysis is 500 mL.

Dirks et al. could indeed show that Sr can be separated with high yields from 250 mL (95.2% +/- 2.5%, N=3) – 500 mL (88.2 +/- 4.3, N=3) water samples with high yields even at sample loading flow rates of 5 – 10 mL/min. Y, Pb and U on the other hand are very well retained, even when a sample of 1L is loaded. Y can be quantitatively removed using 8M HNO₃. Pb and U remain retained even after the Sr elution step and can be eluted using 6M HCl e.g. for Pb-210 determination via α/β discrimination LSC.

Work on the separation of Pb and U on TK100 Resin are ongoing, however, another resin called TK101 Resin allows for facile separation of Pb from other elements.



Elution study, various elements, 1L sample, 100 mL aliquots, TK100 Resin

Main applications




- Direct separation of Ra from water samples
- Direct separation of Pb from water samples
- Direct separation of Sr from water samples

TK101 Resin


Dietz et al. showed that the mechanism of Sr extraction by crown-ethers in ionic liquids strongly depends on the chain-length of the ionic liquid. Long chained ionic-liquids favor liquid-liquid extraction mechanism with high Sr uptake at high nitric acid concentrations whereas short chained ionic liquids introduce a cation exchange mechanism at low acid concentrations, leading to high Sr retention at low pH values. This mechanism further also favors the retention of other divalent cations like Pb, Ba and Ra.

Sr retention then decreases with increasing acid concentrations to a minimum at about 1M HNO₃. At higher HNO₃ concentrations the D_w values increase as expected when the liquid-liquid extraction mechanism becomes predominant. The following graphs show the selectivity of the TK101 Resin.

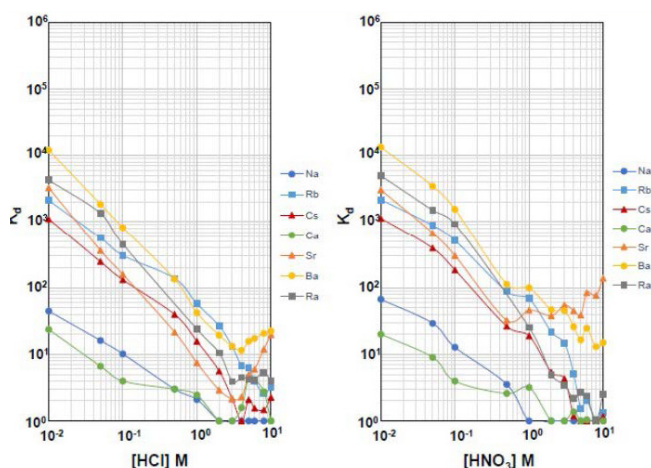

k_D values of selected elements on TK101 Resin in HNO₃.
Data courtesy of Ben Russel (NPL)


As expected, while SR, PB and TK102 Resins show no selectivity for Sr, Ba, Ra at low acid concentrations TK101 Resin does. In dilute HNO₃ as well as in HCl Ba, Ra and Sr are very well retained from ≤ 0.01 M to approx. 0.05M. Their retention decreases significantly as the acid concentration increases though. Sr retention in HNO₃ is an exception as it shows increasing retention at HNO₃ concentrations > 3 M. It should be noted that, while Ra and Ba behave similar at lower acid concentrations, they do show differences at higher acid concentrations, notably at 3M HNO₃, where the k_D Ba is higher than k_D Ra, thus allowing for a Ra/Ba separation.



k_D values of selected elements on TK101 Resin in HNO_3
Data courtesy of Ben Russel (NPL)

Pb is very well retained over the whole HNO_3 concentration range. It is also very well retained from HCl up until approx. 3M HCl. It's retention then decreases very sharply as the HCl increases, making HCl of high concentration suitable for Pb elution.


Out of the elements shown in the graph above only Bi is also retained, particularly from dilute HCl at elevated acid concentrations. It can be very easily removed though, especially using HNO_3 . Lanthanides and actinides are not retained on TK101 not in HCl neither in HNO_3 .

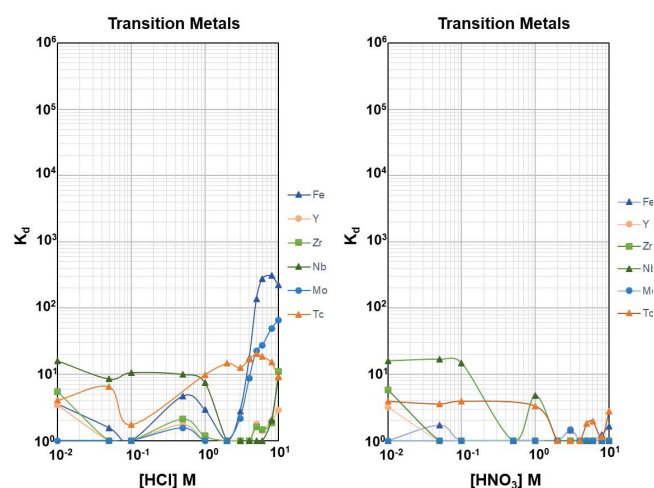

k_D values of selected elements on TK101 Resin in HNO_3
Data courtesy of Ben Russel (NPL)

Out of the tested transition metals only Nb shows some retention at high HCl, all other elements tested show very low k_D values.


The graph hereafter shows the result of an elution study performed with amongst others Th, Ce, Pt, Ir, Ba, Ra and Pb.



Elution study of selected elements on TK101 Resin
Ra data courtesy of Nora Vajda (RadAnal)

Other elements tested than Ba, Ra and Pb are removed during load and rinse with dilute acid (here 0.05M HNO_3). Ra is then eluted with 3M HNO_3 , while Ba and Pb remain retained. Ba is eluted with 8M HNO_3 . Pb is still retained under these conditions and may then be eluted with 6 – 8M HCl or citrate/citric acid.

An elution study performed by Dirks et al. using the TK101 Resin showed that indeed a clean Pb fraction can be obtained applying a similar separation scheme as employed for the TK100 Resin. High Pb yields are obtained even when loading 1L samples or more at flow rates of 5 – 10 mL/min.




Elution study, 1L sample, 100 mL aliquots, TK101 Resin

Main applications

- Direct separation of Pb from water samples
- Ra separation

TK102 Resin

The TK102 Resin is based on the same crown-ether that is also used in the SR and PB Resins.




4,4'-(5'-di-t-butylcyclohexano-18-crown-6)

Other than these resins the TK102 Resin contains a long-chained fluorinated alcohol as diluent. The resin further contains a larger amount of the crown-ether compared e.g. to the SR Resin. Further the organic phase is impregnated onto an inert support containing aromatic groups for increased stability against radiolysis.

The resin was originally optimized for the separation of Ba and Ra, however it also shows very interesting properties with respect to Sr and Pb separation.

The following two graphs show the selectivity of the TK102 Resin for a range of elements in HNO_3 and HCl. The third graph shows the influence of increasing amounts of Na, K and Ca on the Sr retention in 3M HNO_3 .


All D_w shown in these graphs were obtained through ICP-MS measurements.



D_w values of selected elements on TK102 Resin in HNO_3

Pb is very well retained over the whole HNO_3 concentration range. Sr is well retained at elevated HNO_3 concentrations (3 – 10M HNO_3), showing higher Sr D_w values than the SR Resin under these conditions. The same is true for Ba at 3M HNO_3 , TK102 Resin shows stronger Ba retention than SR Resin


Further it is notable that Tl is strongly retained



D_w values of selected elements on TK102 Resin in HCl

As expected, Pb is well retained over a wide HCl concentration range, from dilute HCl up to 2 – 3M HCl. Pb D_w values drop strongly for higher HCl concentrations (≥ 6 M HCl), allowing for its elution under these conditions.

The TK102 Resin retains, to a certain extent similar to the TK400 Resin, a number of elements at very elevated HCl concentrations, including Tl, Sb, Sn, Ga and Nb.



D_w values Sr on TK102 Resin in 3M HNO_3 and in presence of increasing amounts of Na, K and Ca

Na shows very little influence on the Sr retention on the TK102 Resin, even at concentrations up to 1M D_w values for Sr remain high.

Ca is showing a higher impact, nevertheless even at concentrations up to 0.5M Sr shows elevated D_w values.


As expected, K is interfering with the Sr retention very strongly, even concentrations ≥ 0.05 M will lead to a significant decrease in Sr retention.

Just like for the SR Resin, performing a co-precipitation (e.g. with calcium phosphate) to remove K before the actual separation on TK102 Resin is crucial.

The following figures are showing three comparative elution studies on TK102 Resin and SR Resin.

The first example is a typical Pb separation based on loading from 2M HCl, Po removal with dilute HNO_3 and finally Pb elution with citrate.

Both resins are showing very similar elution profiles, TK102 Resin might require a slightly larger elution volume for Pb though. Nevertheless, typically employed elution volumes (e.g. 10 mL) should assure quantitative elution of Pb also from TK102 Resin.


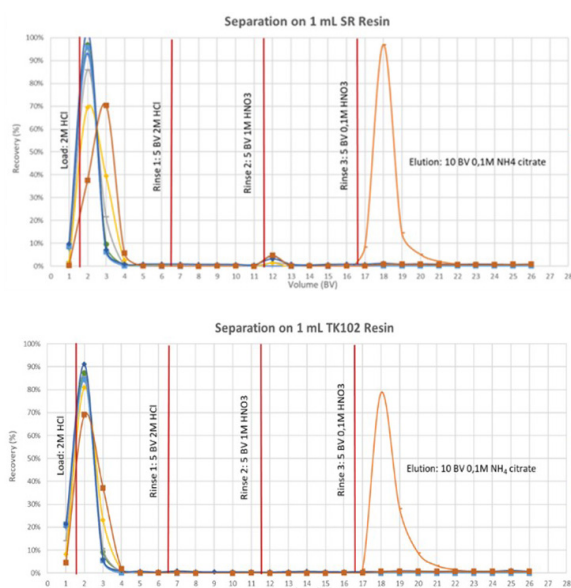


Comparative elution studies, SR and TK102 Resin, Pb separation

The second example is a typical Sr separation based on loading from 3M HNO_3 , rinsing with 8M HNO_3 and 3M HNO_3 /0.1M oxalic acid, and finally Sr elution in 0.05M HNO_3 .

Again, both resins are showing similar elution profiles. One distinct difference being Th, for the TK102 Resin 3M HNO_3 /0.1M oxalic acid rinse is required to remove most of the Th while on SR Resin the majority is already removed with 8M HNO_3 .

Like for the Pb separation Sr elution from TK102 Resin seems to require slightly larger volumes, but here too typically employed elution volumes (10 – 15 mL) seem to assure quantitative Sr elution.




Comparative elution studies, SR and TK102 Resin, Sr separation

The third example shows a comparative Ba/Ra separation elution study. TK102 and SR Resin were both loaded from 3M HNO_3 , then both resins were rinsed with several bed volumes (BV) of 3M HNO_3 .

For both resins Ra is eluted quickly during load and first rinsing steps, while Ba remains retained.

On the SR Resin Ba starts to significantly break through after 6 BV, on the TK102 Resin the Ba retention is distinctively stronger, it starts to very slowly elute after about 8 - 9 BV.

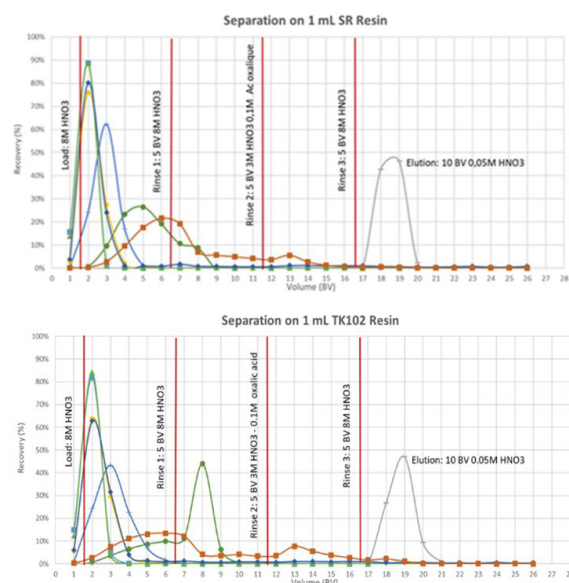

Comparative elution studies, SR and TK102 Resin, Ba/Ra separation

Further the TK102 Resin shows high dynamic capacity for Sr (>40 mg/g) and Pb (>90 mg/g).

Due to the higher hydrophobicity of the diluent employed in the TK102 Resin it also shows significantly (>10 times) less bleeding of organic material, measured as Non-Purgeable Organic Carbon (NPOC), than the SR Resin.

Main applications

- Ra/Ba separation
- Sr separation
- Pb separation

Guard Resin

The Guard Resin is a hydrophobic, highly crosslinked, porous polydivinylbenzene based adsorbent. Due to its high hydrophobicity it will remove certain organic impurities, notably organic impurities that are hydrophobic, more efficiently than e.g. the Prefilter Resin. The Guard Resin is generally used in reversed phase chromatography and solid phase extraction, and for the adsorption of biomolecules of up to 14 kDa. It has a surface area of $> 600 \text{ m}^2/\text{g}$ and a typical porosity in the order of $300 - 500 \text{ \AA}$. The resin shows high mechanical and chemical stability, and it may be used over the whole pH range.

Another application of the Guard Resin is the separation, in combination with the ZR Resin, of Ge-68 from GaNi or GaCo targets. The actual separation of Ge from the target material is performed on two consecutive ZR Resin cartridges. The Guard Resin may then be used in the final step of the purification, namely the conversion of final product Ge-68 from dilute citric acid to dilute hydrochloric acid.

The Guard Resin is TSE/BSE/GMO free..

Main applications



- Removal of organic impurities
- Ge-68 (in combination with ZR Resin)



TK-TcScint Resin

The TK-TcScint Resin is the first of a range of resins based on “Impregnated Plastic Scintillation microspheres” developed by García, Tarancón and Bagán at the University of Barcelona.

This range of new products will be comprised of plastic scintillation microsphere (PSm), supplied by the group at the University of Barcelona, that are impregnated with selective extractants.

The TK-TcScint Resin is, as the name indicates, mainly dedicated to the quantification of Tc-99. The extractant used in its fabrication is Aliquat 336, it further contains small amounts of a long-chained alcohol. Accordingly, its selectivity will generally be very similar to the TEVA Resin.

The figures below (a and b) show SEM pictures of the non-impregnated PSm, and the impregnated




Figure a and b: left - non-impregnated plastic scintillation microspheres (PSm), right - impregnated PSm (TK-TcScint Resin).

Taken from García et al.

microspheres (TK-TcScint Resin), respectively.

The TK-TcScint Resin is generally employed as pre-packed 2 mL cartridges for use with vacuum box systems, or automatized separation equipments based on pump systems

The PSm support employed in the TK-TcScint Resin is itself acting as scintillating medium, this allows for a direct measurement of the Tc-99 retained on the cartridge, no elution and mixing of the eluate with a liquid scintillation cocktail is necessary.

- Gain of time which is particularly interesting in emergency situations
- No mixed liquid radioactive waste
- No Tc elution with HNO_3 of elevated concentration and no evaporation / aliquoting of the eluate
- No cutting of columns or cartridges to push the resin into LSC vials

This has a number of advantages:


Especially the latter two points are interesting in terms of radiation protection when samples of elevated activity are being analyzed.

Ideally the chemical yield is determined via ICP-MS or

ICP-OES using Re as internal standard.

The following graph compares this new approach based on impregnated PSm Resins such as the TK-TcScint Resin with classical methods.

In order to easily handle and avoid contaminating the LSC counter the cartridges should be placed in a

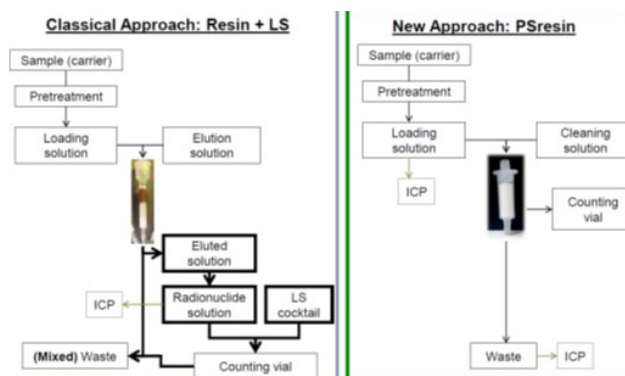

Overview classical radioanalytical method and PS Resin approach. Taken from García et al.


standard 20 mL LSC vial for its measurement.

Typical samples analysed include urine and various types of water samples. In case of surface water samples generally a breakthrough volume of > 200 mL can be achieved using 2 mL cartridges, making this technique not only interesting in emergency situations or as screening tool in decommissioning, but also for use in routine biomedical or environmental monitoring. For water samples the chemical yield is generally >98.8%.

The detection efficiency for Tc-99 obtained with the TK-TcScint Resin is very high, in the order of 89.5(0.6)%, while the background of the standard 2 mL cartridges is low with ~1.09 CPM (obtained in Quantulus™ detector in the high-energy and low-coincident bias configuration).

Further the TK-TcScint Resin cartridges show reproducibly low quench with a mean SQP(E) of 787(7).

The figure below shows typically obtained Tc-99



Liquid Scintillation Spectrum of Tc-99 on TK-TcScint Resin.

Taken from García et al.

The analysis of water samples such as e.g. river and sea water (typically 50 mL) using TK-TcScint Resin cartridges is rather straightforward.

After filtration, if necessary, samples are heated to 90°C for 60 min after addition of a few mL of 30% H₂O₂ to assure that Tc is present as pertechnetate. The solutions are then adjusted to 0.1M HCl using conc. HCl. Once the samples reach room temperature, they are ready for separation.


After loading of the sample the cartridge is typically rinsed successively with 0.1M HCl, 0.1M HNO₃/0.1M HF (only necessary in case Th is expected to be present) and finally water.

These rinses allow eliminating possible interferences while Tc (and the internal standard Re) remain on the cartridge. Load and rinse fractions are combined and analysed for Re content to allow calculating the chemical yield of the separation. The TK-TcScint Resin cartridge can then be directly counted on an LSC counter.

The authors found very good match between expected and measured activities, for the spiked water samples as well as for two spiked MAPEP samples.

Using 50 mL samples and 180 min counting time allowed the authors obtaining a limit of detection of 0.15 Bq.L⁻¹.

As could further be shown by the authors, this method can easily be automatized. In their case they developed their own separation unit called OPENVIEW-AMSS, a modular, vacuum box based equipment. They could show that both, manual and automatized separations allow for obtaining high chemical yields and detection efficiencies, no significant differences were observed when analysing samples in parallel. However, with respect to hands-on time and radiation protection automatization provides significant advantages.

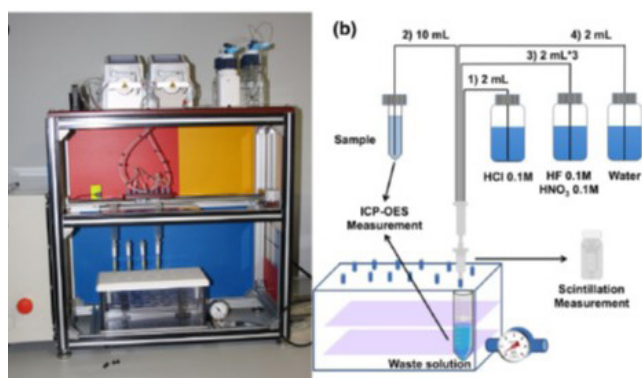

OPENVIEW-AMSS system and scheme of a typical separation of water samples. Taken from Coma et al

Further to the unit developed by the authors the TK-TcScint Resin cartridges are also compatible with commercially available equipment such as the Hidex Q-Are 100.

Besides water samples urine samples were also analysed using TK-TcScint Resin cartridges.

With respect to their higher matrix load this kind of samples requires a thorough sample pre-treatment. The described method is based on 100 mL urine samples that are first wet-ashed using conc. HNO₃, followed by an additional ashing step in a muffle furnace at 550°C. The obtained ash is then dissolved in 3 mL of conc. HNO₃ and diluted to 100mL using deionized water. To assure Tc is present as pertechnetate the solutions are heated, after addition of a few mL hydrogen peroxide, to 90°C for 60min. As described before, Re was used as internal standard.

By analysing spiked urine samples the authors could show that accurate results can be obtained using the impregnated PSm approach. A minimum detectable activity (MDA) of 0.036 Bq.L⁻¹ for 100mL samples and 24h counting was reported.

Further to the analysis of Tc-99, PSm Bagán et al. showed that Aliquat 336 impregnated resins may also be used for the analysis of [¹⁴C]SCN⁻ used as radiotracer for study of oil reservoir dynamics.

With respect to the selectivity of the Aliquat extractant, the compound giving TEVA Resin its selectivity, a use of the TK-TcScint Resin cartridges for the screening of other radioelements such as e.g. Pu isotopes or Po-210

Main applications




- Separation and LSC measurement of technetium


UPCOMING NEW PRODUCTS

TK222 Resin



The TK222 Resin is based on a mixture of a branched diglycolamide and a phosphine oxide. It additionally contains a small amount of a long-chained alcohol. Further, the organic phase is impregnated onto an inert support containing aromatic groups for increased stability against radiolysis. TK222 Resin is currently mainly being tested for use in Ac-225 purification, and in the purification of lanthanides, especially heavy lanthanides such Lu-177. Some first technical information is shown below.



D_w values of selected elements on TK222 Resin in HNO_3




D_w values of selected elements on TK222 Resin in HCl



Comparative elution study: Lu purification on TK221 (t grade) and TK222 (t grade) Resins. ICP-MS data.

Weight distribution ratio of Ac on TK221 and TK222 resins



D_w values of Ac of TK221 and TK222 Resins in HCl (data courtesy of N. Vajda, Radanal)

Main applications



- Ac Purification
- Lu-177 Purification

Samples of the TK222 Resin are available upon request at contact@triskem.fr

CU Sheets

The upcoming new CU Sheets are comprised of a routinely used iTLC paper impregnated with the same extractant that is also used in the CU Resin. The graph below compares the performance of these new CU Sheets with other routinely used TLC papers.

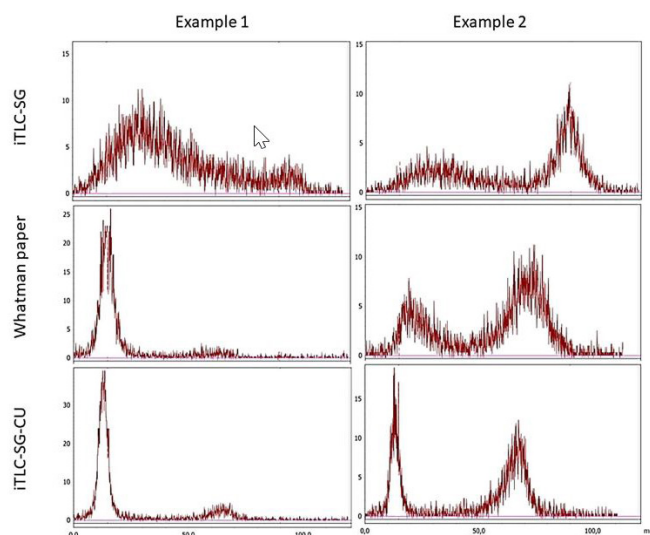


Figure 1. TLC scans of $[^{61}\text{Cu}]\text{Cu-NOTA-octreotide}$ spotted on: top, iTLC-SG; middle, Whatman

TLC scans of $[^{61}\text{Cu}]\text{Cu-NOTA-octreotide}$ spotted on: top, iTLC-SG; middle, Whatman paper; bottom, extractant-impregnated iTLC-SG (CU Sheets). Example 1 notes elevated levels of unlabelled ^{61}Cu , while example 2 notes comparable levels of labelled to unlabelled ^{61}Cu

Data courtesy of Svedjehed et al.: "New extractant-impregnated iTLC-SG paper facilitates improved TLC analysis for Cu radiolabelled peptides", poster presented at TERACHEM 2022, 14 – 17 September 2022, Bressanone (Italy). Poster available online on our website.

Samples of the CU Sheets are available upon request at contact@triskem.fr. Please also contact us in case you are interested in other types of 'Sheets'


Main applications



- QC of Cu radiolabelled compounds

Impregnated membrane

A new range of impregnated membrane filters, based i.e. on the extractants employed in TK201 Resin, TK100 Resin, CL Resins,... will be available soon. The membrane filters will be available in two sizes, 47mm and 25mm. Their main applications will be the separation of analytes from water samples using a filtration unit and passive sampling via DGT (Diffusive Gradients in Thin Films).



Main applications




- Tc-99 in water samples (TK201)
- Radioiodine in water (CL Resin)
- Pb in water samples (TK100)
- Pb, Sr, Zn via DGT (TK100)



SPECIALTY ION EXCHANGE RESINS

TK202 Resin

The TK202 Resin is based on Polyethyleneglycol (PEG) groups, with high molecular weight, that are covalently bound onto a polymer support.




PolyEthyleneGlycol (PEG).

The TK202 Resin is based on an aqueous biphasic system (ABS) extraction mechanism with the covalently bound PEG acting as solid separation support. In presence of aqueous solutions with high ionic strength and high content of water-structuring (kosmotropic) anions like SO_4^{2-} , CO_3^{2-} , OH^- , as well as MoO_4^{2-} or WO_4^{2-} , it will extract chaotropic ions, according to Spear et al. notably TcO_4^- and ReO_4^- , while other non-chaotropic elements will not be retained, molybdenum being an important example. Accordingly, Tc (and Re) retention will improve with increasing concentration of these anions.


The following graph shows D_w values for Tc, Re and Mo on TK202 Resin at increasing OH^- concentrations.

Ideally the NaOH concentration should be between 5 and 7M NaOH during load and rinse, as Tc (and



D_w values for Tc, Re and Mo on TK202 Resin, at varying NaOH concentrations. Re retention is highest while Mo retention is very low.

As mentioned before, MoO_4^{2-} itself is a kosmotropic anion. Accordingly, increasing its concentration will lead to higher Tc (and Re) retention in ABS systems like the TK202 Resin, as shown below. A



D_w values for Tc in 5M NaOH using 40 mg TK202 Resin, increasing amounts of Mo. Data taken from Cieszykowska et al.

distinct increase of the Tc retention with increasing amounts of Mo is observed.

This is particularly relevant in case of the separation of Tc from elevated amounts of Mo (e.g. irradiated Mo targets).

Cieszykowska et al. estimated from column studies that 6 to 8g of Mo per g of TK202 Resin allow obtaining high Tc recovery (> 90%). Further increasing the amount to 12g Mo/g of resin lead to a decrease of the Tc recovery to ~82% in their experiments.

The retained Tc and Re can then be eluted with water as the ABS systems breaks down, due to the low concentration of kosmotropic anions, under these conditions.

As mentioned, one potential application of the TK202 Resin is the separation of Tc-99m from irradiated Mo targets. Accordingly, its high selectivity for Tc over Mo, and the fact that the presence of elevated amounts of Mo in solution increases the Tc retention, makes the TK202 Resin particularly suitable for this type of applications.

Indeed, besides the production of Mo-99 for the fabrication of Mo-99/Tc-99m generators via U-235 fission there are a number of other ways to produce

- Neutron activation of Mo-98 via (n, γ) reactions (Mo-98 (n, γ) Mo-99), preferably performed in a reactor with high neutron flux.
- Photon-induced (γ , n) reaction of Mo-100 (Mo-100 (γ , n) Mo-99) using photons (γ) obtained through irradiation of heavy targets (converter) e.g. with electron beams.
- Direct Tc-99m production on a cyclotron using Mo-98 targets (Mo-98 (p, 2n) Tc-99m). This latter method represents, with respect to the short half-life of Tc-99m, certain logistical challenges and will generally rather allow for supplying users close to the production facility. This method requires a clean, and very rapid, separation of the produced Tc-99m from the target material.

The first two described methods tend to result in Mo-99 of limited specific activity, especially compared to Mo-99 obtained from U fission. Accordingly using them e.g. in alumina column based generator systems will, due to the generally limited Mo capacity of these columns, result in rather lower activity Mo-99/Tc-99m generators.

In such cases employing a resin, such as the TK202 Resin, to extract the Tc-99m originating from Mo-99 decay while letting Mo pass through ("inverted generator") is often a preferred option.


It should be noted that in all three cases the recovery and recycling of the enriched Mo is of very high importance due to the pricing and limited availability of the target material.

The production methods described above all require the use of a resin with high selectivity for Tc over large amounts of Mo. Ideally, as the Mo targets are very frequently dissolved in NaOH solutions of elevated concentration, the resin should show this selectivity under these conditions.

This is the case for the TK202 Resin. As indicated before, Tc may then be recovered using water, although further separation steps will be necessary to adjust pH and Na⁺ concentration of the final product.

Initial elution studies using Re instead of Tc confirmed the high selectivity for Re (and, as could be confirmed in separate tests, also Tc) over Mo.


The graph on the right shows an elution study performed with trace amounts of Mo and Re. As it can be seen, a clean separation of both elements is obtained. Mo is removed during load and following rinses (both may be performed with 5 – 7M NaOH), while Re elutes in a small water volume.



Elution study, trace amounts of Mo and Re on a 2 mL TK202 Resin cartridge, load and rinse at 1 BV/min, elution at 0.25 BV/min.

As the general selectivity could be confirmed further tests were performed using larger amounts of Mo.

The elution study below shows the separation of traces of Re from 2g of Mo, as e.g. typically required in case of Tc-99m production from Mo-98 irradiation in a cyclotron, as described e.g. by Bénard et al.




Elution study, separation of trace Re and 2g Mo on a 2 mL TK202 Resin cartridge, load and rinse at 1 BV/min, elution at 0.25 BV/min.

It should be noted that purging the resin, e.g. with air, after the rinse and before its elution with water, to remove NaOH from the cartridge/column, is of high importance to reduce the Na⁺ and OH⁻ load of the final Tc/Re fractions.

It could further be shown that lower flow rates during elution of the TK202 Resin will result in narrower elution peaks, and thus lower elution volumes.

As discussed previously, the TK202 Resin may also be used to extract Tc-99m from Mo-99 decay present in an alkaline solution. In such cases much larger Mo targets are generally irradiated.

With respect to this, the separation of trace of Re from 100g Mo was tested. As shown below a clean separation of Mo and Re could be obtained here, too. Nevertheless, with respect to the very large amount of Mo present, an additional purification of the obtained Tc will be required.



Elution study, separation of trace amounts of Re and 100g Mo on a 75 mL TK202 Resin cartridge, load at 0.5 BV/min, rinse at 1 BV/min, elution at 0.2 BV/min

Elution study, separation of trace amounts of Re and 100g Mo on a 75 mL TK202 Resin cartridge, load at 0.5 BV/min, rinse at 1 BV/min, elution at 0.2 BV/min.

Methods for the separation of Tc from larger Mo amounts (e.g. $\geq 200\text{g}$) are currently being tested.

As shown e.g. by Bénard et al., one convenient option for this additional Tc purification is the use of a cation exchange resin (for Na^+ removal and pH adjustment to below pH 7), followed by an alumina cartridge (for Re/Tc concentration and further Mo removal).


Especially for the cation exchange cartridge it is important to adjust the size of the cartridge to the amount of Mo previously present in the sample/and so the size of the TK202 Resin cartridge employed.

For the size of the alumina cartridge on the other hand the amount of residual Mo will be a decisive parameter.

The graph below shows the continuation of the 2g Mo separation test shown before.

The obtained Re fractions (E1 – E4) were combined and loaded through a C8 cation exchange resin cartridge which was then rinsed with water. The load fractions and the first rinse were collected, analyzed, and then combined for the final step of the separation, as they contain all the Re (or Tc).

Continuation of the separation of Re from 2g Mo (see above). Na^+ removal and pH adjustment of Re fractions on 2 mL C8 Resin cartridge, load and rinse at 2 BV/min.




Continuation of the separation of Re from 2g Mo (see above). Na^+ removal and pH adjustment of Re fractions on 2 mL C8 Resin cartridge, load and rinse at 2 BV/min

As stated before, at this stage the Re fraction should be below pH 7 (typically 3 – 5) and largely free of Na^+ cations.

It could be shown that under these conditions, acidic alumina will retain Re/Tc (and Mo). A 0.9% NaCl solution then allows eluting Re/Tc in a small volume (2 – 3 BV) while Mo remains very strongly retained, thus further improving the purity of the recovered Re/Tc.

The indicated air purge is not necessary in case of the AlOxA Resin (acidic alumina).




Re concentration, purification and conversion to 0.9% NaCl solution on 1 mL AlOxA Resin at 2 BV/min

This further has the advantage of allowing to obtain the Tc in the same matrix (0.9% NaCl) as delivered by a Mo-99/Tc-99m generator.

Overall, in the cold tests Re recoveries in the order of $>90\%$ could be obtained.

A schematic overview of the suggested separation method is given below. The method may be applied for the separation of Tc from Mo targets of various sizes, cartridge/column volumes will need to be adjusted accordingly.

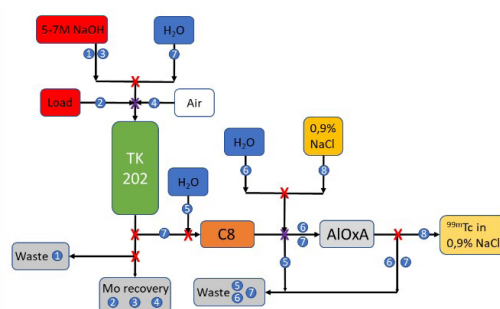

- 1 Pre-cond. TK202 – 5-7M NaOH \rightarrow alkaline waste
- 2 Load Mo/Tc on TK202 \rightarrow Mo recovery
- 3 Rinse TK202 – 5-7M NaOH \rightarrow Mo recovery
- 4 Purge TK202 – Air \rightarrow Mo recovery
- 5 Pre-cond. C8 – H_2O \rightarrow Aq. waste
- 6 Pre-cond. AlOxA – H_2O \rightarrow Aq. waste
- 7 Elute Tc from TK202 on C8 then on AlOxA – « H_2O »
- 8 Elute Tc from Al_2O_3 – 0,9% NaCl \rightarrow Tc recovery

Schematic overview, Tc separation from Mo.


Further to the TK202 Resin TrisKem also supplies C8 Resin, AlOxResin.

All resins are available in various columns and/or cartridges of different sizes (depending on the size of the Mo target).

Please contact us for further information.

Besides the described radiopharmaceutical use the TK202 Resin may also be employed in radioanalytical applications, notably in the analysis of Tc-99 in samples that were solubilized via alkaline fusion.

In such cases the solubilized samples (e.g. concrete samples resulting from decommissioning work) may, after removal of insoluble material, be adjusted to 5 – 7M NaOH and then passed through TK202 Resin to separate Tc.



Re separation from selected elements on 2 mL TK202 Resin cartridge, load and rinse at 1 BV/min, elution at 0.25 BV/min.

In order to further increase the purity of the obtained Tc fraction it might be passed, as described above, through a C8 Resin, and potentially even AlOxResin.

Main applications

- Separation of technetium
- Separation of rhenium



Cs Resins

Both resins, AMP-PAN and KNiF-PAN have been developed by Dr. Šebesta from the Czech Technical University in Prague. Like the MnO_2 -PAN resin both resins are based on very fine and selective inorganic materials embedded in an organic matrix based on polyacrylnitrile (PAN) in order to improve their mechanical characteristics. The active components are the widely employed ammonium phosphomolybdate (also Ammonium MolybdoPhosphate, AMP) and potassium nickel hexacyanoferrate(II) (also potassium Nickel FerroCyanate, KNiFC).


Both resins are used for the concentration and separation of Cs from various liquid samples.

Ammonium phosphomolybdate is an inorganic ion exchanger known for its high selectivity for Cs even at elevated acid concentrations, quick kinetics and radiation stability.

Its high selectivity for Cs even under harsh chemical conditions and high levels of radioactivity make the AMP-PAN resin a candidate resin for the treatment of radioactive waste solutions. Brewer et al. tested the resin for the removal of Cs-137 from real and simulated acidic high-active liquid radioactive waste containing high amounts of potassium and sodium.

AMP-PAN's robustness against high salt concentrations also makes it interesting for use in environmental analysis, especially the analysis of Cs-134/7 in sea water. Kamenik et al. evaluated AMP-PAN and KNiFC-PAN resins for use in Cs-134/7 analysis in sea water samples.

The authors passed 100L of acidified seawater samples (in case of KNiFC-PAN unacidified seawater samples were tested as well) through 25 mL beds of AMP-PAN or KNiFC-PAN resin at flow rates up to 300 mL.min⁻¹ allowing for processing 100L samples in less than 6h. Stable Cs was added to the seawater samples to allow for the determination of the chemical yield e.g. via ICP-MS.



Ammonium MolybdoPhosphate [AMP] and potassium Nickel FerroCyanate [KNiFC]

After loading resins were rinsed from the columns, dried and measured by gamma spectrometry in Petri dish geometry. Chemical yields obtained are generally high (>90%), KNiFC-PAN showing slightly higher yields for the acidified seawater samples than AMP-PAN resin and comparable chemical yields for acidified and non-acidified seawater samples. Higher flow rates were tested for the processing of non-acidified sea water samples on KNiFC-PAN resin; even at a flow rate of 470 mL.min⁻¹ Cs yield is still greater than 85%.

KNiFC-PAN resin was further used for the determination of Cs isotopes in milk and urine.

Main applications



- Concentration and separation of Cesium

MnO₂-PAN Resin

The analysis of Ra isotopes in water samples is becoming more and more important. To meet existing requirements on detection limits, especially for Ra-228, elevated samples volumes have to be used for analysis. MnO₂ Resin allows to preconcentrate Ra isotopes efficiently from water samples, drinking water as well as sea water.

MnO₂ Resin is currently used with LN Resin and DGA Normal resin in a method developed by Sherrod Maxwell of Westinghouse Savannah River. In his method the MnO₂ is used to pre-concentrate Ra from 1 to 1.5L water samples, with 1.25 g/L of MnO₂ resin used per sample.

Ra is then eluted and loaded (in case Ra-228 is to be determined after a minimum of 36 hours for Ac-228 ingrowth) onto DGA, Normal Resin (retention/separation of Ac-228). Ac-228 is eluted from the DGA Resin and finally micro-precipitated with CeF₃ and counted via GPC; the precipitated source can

be used for gravimetric yield determination. Ra-226 can be determined, directly or after additional clean-up via LN Resin, by BaSO₄ micro-precipitation and alpha spectrometry.


TrisKem International is providing the MnO₂-PAN resin (G2 Resin) developed by Dr. Šebesta (CVUT).

It consists of very fine MnO₂ particles embedded into a modified polyacrylonitrile (PAN) binding polymer offering a very stable MnO₂ resin with a very high surface area.

Main applications



- Determination of Ra-226/8 in water samples




Absorption of Ba-133 on MnO₂ Resin

SAMPLE PREPARATION

Nucfilm Discs

Recent improvements in the fabrication of MnO_2 layers by Dr. Heinz Surbeck (Nucfilm GmbH) now allow the fabrication of selectively adsorbing MnO_2 coated as a thin film onto the surface of a polyamide disc. These coated substrates are available as Ra Nucfilm Discs. Due to their high selectivity for Ra the discs allow the direct determination of Ra isotopes in water samples without applying additional radiochemical separation methods.



Alpha spectrum of a radium adsorbing thin film exposed to a Portuguese mineral water:

The discs are contacted with the untreated water samples (pH 4 – 8, typical volume = 100 mL) under stirring for 6h. Under these conditions the Ra extraction is typically greater than 90%. The dried disc can then be measured with a solid state alpha detector.

The energy resolution of the obtained sources is very good, typically FWHM in the order of 30 to 40 keV are obtained. The analysis of a 100 mL sample (counting time $t = 80000$ s, 900 mm^2 Si-detector at 10 mm distance) typically results in a detection limit (LLD) of 5 mBq.L^{-1} for Ra-226.

Main applications


- Determination of Ra-226 in water samples

Discs for alpha spectrometry source preparation

TrisKem is providing stainless steel discs for electrodeposition source preparation. Silver and nickel discs as well as an auto-deposition kit are available for the particular case of polonium auto-deposition.



Ra Nucfilm Disc




Nickel Disc





Silver Disc

Auto-deposition KIT AC 05 ADK


Instruction for Use



(1) Plastic rotative unit, (2) Flat circular magnet Ring, (3) Disk, (4) Ring, (5) Clamping ring, (6) Retaining clip



Insert (2) Flat circular magnet Ring into (1) Plastic rotative unit then the (3) Disk and the (4) Ring



Place the (6) Retaining clip in the (5) Clamping ring



The system is ready for deposition in a beaker on stirring plate



Tighten the (5) Clamping ring in the (1) Plastic rotative unit

REFERENCES

- J. L. Cortina and A. Warshawsky Ion Exchange and Solvent Extraction; Marinsky, J.A., Marcus, Y., Eds.; Marcel Dekker: , 1997; Vol. 13, p.195.
- M. L. Dietz, E. P. Horwitz, and A. H. Bond, » Metal in Separation and Preconcentration: Progress and Opportunities, Bond, A. H., Dietz, M. L., , R.D., Eds.; ACS Symposium Series 716, ACS, , 1999, pp. 234-250.
- E. P. Horwitz, R. Chiarizia, and M. L. Dietz, Solvent Extr. Ion Extr. 1992, Vol. 10, pp. 313-336.
- E. P. Horwitz, M. L. Dietz, R. Chiarizia, H. Diamond, S. L. Maxwell, III, and M. R. Nelson, Anal. Chim. Acta 1995, Vol. 310, pp. 63-78.
- E. P. Horwitz, R. Chiarizia, and M. L. Dietz, Reactive and Functional Polym. 1997, Vol. 33, pp. 25-36.
- E. P. Horwitz and C. A. A. Bloomquist, J. Inorg. Nucl. Chem. 1972, Vol. 34, pp. 3851-3871.
- E. P. Horwitz and C. A. A. Bloomquist, J. Inorg. Nucl. Chem. 1973, Vol. 35, pp. 271-284.
- E. P. Horwitz, M. L. Dietz, R. Chiarizia, and R. C. Gatrone and A. M. Essling, R. W. Bane, and D. Graczyk, Anal. Chim. Acta 1992, Vol. 266, pp. 25-37.
- E. P. Horwitz, R. Chiarizia, M. L. Dietz, H. Diamond, and D. M. Nelson, Anal. Chim. Acta 1993, Vol. 281, 361-372.
- E. P. Horwitz and C. A. A. Bloomquist, J. Inorg. Nucl. Chem. 1975, Vol. 37, pp. 425-434.
- E. P. Horwitz, M. L. Dietz, S. Rhoads, C. Felinto, N. H. Gale and J. Houghton, Anal. Chim. Acta 1994, Vol. 292, pp. 263-273.
- W. C. Burnett, D. R. Corbett, M. Schultz, E. P. Horwitz, R. Chiarizia, M. Dietz, A. Thakkar, and M. Fern, J. Radioanal. Nucl. Chem. 1997, Vol. 226, p. 121.
- Horwitz E.P., McAlister D.R., Bond A.H., Barans R.E., Solvent Extrac. Ion Exch., 23, 219 (2005).
- Horwitz E.P., Bond A.H., Barans R.E., McAlister D.R., 27th Actinide separations Conferences, (2003).
- Moon D.S., Burnett W.C., Nour S., Horwitz P., Bond A., Applied Rad. Isot., 59, 255 (2003).
- Maxwell, S.L., presented at Eichrom's North American Users' Meeting, , May 3, 2005, see www.eichrom.com.
- Cahill D. F., Peedin L. M., presented at 41st Annual Conference on Bioassay, Analytical and Environmental Chemistry, Eichrom workshop, Boston, MA - USA
- Esser B.K. et al., Anal. Chem., Vol.66, 1736 (1994)
- McAlister D., Horwitz E.P., Solvent Extrac. Ion Exch, 25 (6), 757-769 (2007)
- A. Zulauf, S. Hoppel, M. B. Mokili et al., J. Radanal Nucl Chem, 286(2), 539-546
- P E Warwick, A Zulauf, S Hoppel, I W Croudace, presented at the 11th ERA Symposium, 16/09/2010, Chester (UK), see www.triskem.com
- C. Dirks, B. Scholten, S. Hoppel et al., J Radioanal. Nucl. Chem, 286 (2010) 671-674
- C. Dirks, S. Hoppel, presented at the Triskem International users group meeting, 14/09/2010, Chester (UK), see www.triskem.com
- Chiarizia, R., Sep. Sci. Technol., 32, 1997, 1 - 35
- Kim G., Burnett W.C., Horwitz E.P., Anal. Chem., 72, 2000, 4882-4887
- Shaw D.R. et al., JOM, July 2004, 38 - 42
- Hines, J.J.; et al, Sep Sci Technol, 30(7-9), 1995, 1373 - 1384
- Surbeck H., presented at ICRM Conference on Low Level Radioactivity Measurement Techniques 18-22nd October 1999, Mol, Belgium, see www.nucfilm.com
- Mendes M, Aupiais J, Jutier C, Pointurier F. Anal Chim Acta. 2013 May 30;780:110-6
- Horwitz E.P., Dietz M.L., Rhoads S., Felinto C., Gale N.H., Houghton J.; Analytica Chimica Acta, Vol.292, p263-273 (1994)
- Nottoli E, Bienvenu P, Labet A, Boulès D, Arnold M, Bertaux M. Appl Radiat Isot. 2014 Apr;86:90-6. doi: 10.1016/j.apradiso.2014.01.010.
- Horwitz P, McAlister D. Old Separations on New Resins and New Separations on Old Resins. RRMCM, Destin, FL 2008
- Sebesta F, Stefula V (1990) Composite ion exchanger with ammonium molybdophosphate and its properties. J Radioanal Nucl Chem 140(1):15 - 21
- Brewer et al. (1999). Czechoslov J Phys 49(S1):959-964
- Kamenik et al. (2012) J Radioanal Nucl Chem. DOI 10.1007/s10967-012-2007-4
- Kamenik J et al. (2009) Long term monitoring of Cs-137 in foodstuffs in the Czech Republic. Appl Radiat Isot 67(5):974-977
- Bartuskova et al. (2007) Ingestion doses for a group with higher intake of Cs-137.IRPA regional congress for Central and Eastern Europe, Brasov, Romania
- E. P. Horwitz, M. L. Dietz, R. Chiarizia, H. Diamond, S. L. Maxwell, III, and M. R. Nelson, Anal. Chim. Acta 1995, Vol. 310, pp. 63-78.
- Mark L. Dietz, Julie A. Dzielawa, Ivan Laszak, Blake A. Young and Mark P. Jensen: „Influence of solvent structural variations on the mechanism of facilitated ion transfer into room-temperature ionic liquids”, Green Chemistry, 2003, 5, 682-685
- Dirks et al.: “On the development and characterisation of an hydroxamate based extraction chromatographic resin”. Presented at the 61st RRMCM, October 25th - 30th, 2015, Iowa City, IA, USA
- A. Bombard et al. “Technetium-99/99m New Resins Developments For Separation And Isolation From Various Matrices”, presented at the ARCEBS 2018, 11-17/11/18 - Ffort Raichak (India)
- S. Hoppel: “An overview over some new extraction chromatographic resins and their application in radiopharmacy” presented on the 4th of June 2019 at the 102nd Canadian Chemistry Conference and Exhibition (CCCE 2019) in Quebec City, QC
- S.K. Spear et al., Ind. Eng. Chem. Res., 2000, 39, 3173 - 3180, <https://doi.org/10.1021/ie990583p>
- I.Cieszykowska et al.: “Separation of 99mTc from low specific activity 99Mo”, poster ID 195 presented at the ISTR 2019, October 28 - November 1, Vienna, Austria
- IAEA Nuclear Energy Series, No. NF-T-5.4.: “Non-HEU Production Technologies for Molybdenum-99 and Technetium-99m”, INTERNATIONAL ATOMIC ENERGY AGENCY, Vienna, 2013
- F. Bénard et al, Journal of Nuclear Medicine, 2014, <https://doi.org/10.2967/jnumed.114.143834>
- C. Dirks et al., Presented at the 61st RRMCM, October 25th - 30th, 2015, Iowa City, IA, USA
- S. Hoppel: “An overview over some new extraction chromatographic resins and their application in radiopharmacy”, Version 12/06/2021, https://www.triskem-international.com/scripts/files/60c4a63e7a4475.44279512/tki_rp_210612.pdf, accessed on 15/07/2021
- J. P. Holland et al., Nucl Med Biol., 36(7), 2009, 729-739; doi:10.1016/j.nucmedbio.2009.05.007
- Nair M, et al., Eur J Nucl Med Mol Imaging. 2017;44(Suppl 2):S119-956.
- Stefano Riga et al., Physica Medica, Volume 55,2018, 116-126. <https://doi.org/10.1016/j.ejmp.2018.10.018>
- Rodnick, M.E. et al., EJNMMI radiopharm. chem. 5, 25 (2020). <https://doi.org/10.1186/s41181-020-00106-9>
- Thisgaard, H. et al., EJNMMI radiopharm. chem. 6, 1 (2021). <https://doi.org/10.1186/s41181-020-00114-9>
- V. Radchenko et al., Journal of Chromatography A, Volume 1477, 2016, 39-46, <https://doi.org/10.1016/j.chroma.2016.11.047>.
- Mario Malinconico et al., Journal of Nuclear Medicine May 2018, 59 (supplement 1) 664. https://jnm.snmjournals.org/content/59/supplement_1/664
- Coma et al., Journal of Radioanalytical and Nuclear Chemistry (2019) 321:1057-1065. <https://doi.org/10.1007/s10967-019-06659-7>
- Barrera et al., Analytica Chimica Acta 936 (2016) 259-266. <https://doi.org/10.1016/j.aca.2016.07.008>
- Tarancon et al. “A new plastic scintillation resin for single-step separation, concentration and measurement of 99Tc”, presented at the NRC9 (29/08/16 - 2/09/16, Helsinki, Finland)
- Hidex eBook “Liquid Scintillation Measuring Procedures: New Developments” <https://hidex.com/ebooks/liquid-scintillation-measuring-procedures/measuring-procedures/radionuclides-from-nuclear-fission-activities/2-3-14-tc-by-rad-disk-and-psresins/>
- J. Garcia & A. Tarancon, “Radionuclide determinations with PS Resin MASS WaterRadd”, presented at the European Users Group Meeting in Cambridge (UK) - 21/09/2018, https://www.triskem-international.com/scripts/files/5bae2550c30ed4.50583030/11_j-garcia_a-tarancon_radionuclide-determinations-with-ps-resin_mass_waterradd.pdf
- H. Bagán et al., Analytica Chimica Acta, 736, 2012, 30-35, <https://doi.org/10.1016/j.aca.2012.05.045>

Products	Applications*
CL Resin	Cl-36/I-129, I removal from effluents, Ag
CS Resins (AMP-PAN and KNiFC-PAN)	Cs-134/7
CU Resin	Cu
MnO ₂ -PAN	Ra-226/8
TBP Resin	Sn, Zr, Actinides, Sc
TK100 Resin	Sr, Ra, Pb (direct separation)
TK101 Resin	Pb, Ra (direct separation)
TK102 Resin	Sr, Pb, Ra/Ba separation
TK200 Resin	Ga-67/8, Actinides
TK201 Resin	Tc, Cu, Pu
TK202 Resin	Tc, Re from alkaline samples
TK221 Resin	Actinides, Lanthanides separation and purification (e.g. Lu-177), Ac-225
TK225 Resin	Lanthanides removal from acidic effluents
TK211/212/213 Resins	Lanthanide separation (e.g. nca Lu-177, nca Tb-161)
TK400 Resin	Pa, Fe, Ga, Nb, Mo
TK-TcScint	Tc separation and LSC measurement
ZR Resin	Zr, Ga, Ge, Ti, Mo, Nb
Guard Resin	Removal of organic impurities, Ge-68
DGA Sheets	Quality control of Ra-223, Pb-212, Ac-225/Bi-213, Ge-68/Ga-68
Ra Nucfilms discs	Ra-226
Discs	Source preparation for alphaspectrometry
Autodeposition kit	Source preparation for alphaspectrometry
LSC consumables	LLSC vials

*the main applications are shown in orange

Upcoming new products :
TK222 Resin, CU Sheets, TK-SrScint,...

TrisKem International

3, Rue des Champs Géons – 35170 Bruz – FRANCE

Tel +33 (0)2 99 05 00 09 – Fax +33 (0)2 23 45 93 19 – www.triskem.com – email : contact@triskem.fr

SAS au capital de 100.000 euros – SIRET 493 848 972 00029 – APE2059Z – TVA intra communautaire FR65 493 848 972



V_0324_W